

11-2019

Forensic Evaluation of 6-Dye Chemistry Kit Composed Of 23 Loi with Casework Samples

Naeema Saleh Al Janaahi

Follow this and additional works at: https://scholarworks.uaeu.ac.ae/bio_theses



Part of the [Biotechnology Commons](#), and the [Molecular Biology Commons](#)

Recommended Citation

Al Janaahi, Naeema Saleh, "Forensic Evaluation of 6-Dye Chemistry Kit Composed Of 23 Loi with Casework Samples" (2019). *Biology Theses*. 20.
https://scholarworks.uaeu.ac.ae/bio_theses/20

This Thesis is brought to you for free and open access by the Biology at Scholarworks@UAEU. It has been accepted for inclusion in Biology Theses by an authorized administrator of Scholarworks@UAEU. For more information, please contact fadl.musa@uaeu.ac.ae.

UAEU



جامعة الإمارات العربية المتحدة
United Arab Emirates University

United Arab Emirates University

College of Science

Department of Biology

FORENSIC EVALUATION OF 6-DYE CHEMISTRY KIT
COMPOSED OF 23 LOCI WITH CASEWORK SAMPLES

Naeema Saleh Al Janaahi

This thesis is submitted in partial fulfilment of the requirements for the degree of
Master of Science in Molecular Biology and Biotechnology

Under the Supervision of Prof. Synan Abu-Qamar

November 2019

Declaration of Original Work

I, Naeema Saleh Al Janaahi, the undersigned, a graduate student at the United Arab Emirates University (UAEU), and the author of this thesis entitled "*Forensic Evaluation of 6-Dye Chemistry Kit Composed of 23 Loci with Casework Samples*", hereby, solemnly declare that this thesis is my own original research work that has been done and prepared by me under the supervision of Professor Synan Abu-Qamar in the College of Science at UAEU. This work has not previously been presented or published, or formed the basis for the award of any academic degree, diploma or a similar title at this or any other university. Any materials borrowed from other sources (whether published or unpublished) and relied upon or included in my thesis have been properly cited and acknowledged in accordance with appropriate academic conventions. I further declare that there is no potential conflict of interest with respect to the research, data collection, authorship, presentation and/or publication of this thesis.

Student's Signature: _____



Date: _____

5/1/2020


Approval of the Master Thesis

This Master Thesis is approved by the following Examining Committee Members:

- 1) Advisor (Committee Chair): Prof. Synan AbuQamar
Title: Professor
Department of Biology
College of Science

Signature  Date 14/11/2019

- 2) Member: Dr. Ranjit Vijayan
Title: Associate Professor
Department of Biology
College of Science

Signature  Date 14/11/2019

- 3) Member (External Examiner): Dr. Mohammad Shahid Nazir
Title: Associate Professor
College of Biotechnology
Institution: University of Modern Science, UAE


Signature  Date 14/11/19

This Master Thesis is accepted by:

Dean of the College of Science: Professor Ahmed Murad

Signature  Date 27/12/2019

Dean of the College of Graduate Studies: Professor Ali Al-Marzouqi

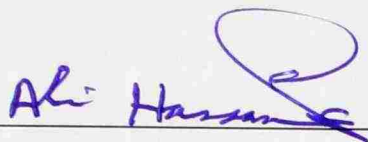Signature  Date 20/1/2020

Copy 7 of 7

Copyright © 2019 Naeema Saleh Al Janaahi
All Rights Reserved

Advisory Committee

1) Advisor: Prof. Synan AbuQamar

Title: Professor

Department of Biology

College of Science

2) Co-advisor: Dr. Rashed Alghafri

Title: Associate Professor

General Department of Forensic Sciences and Criminology

Dubai Police, UAE

Abstract

Short Tandem Repeats (STRs) are short nucleotide sequence repeats consisting of 2-8 base pairs (bp), representing approximately 3% of human DNA. Markers of STRs have been widely used as genetic markers in forensic DNA analysis and have proven to be an extremely discriminating method for human identification in forensics. The main objective of this research was to evaluate a six-dye STR multiplex assay (Virifiler™ Plus) composed of 23 autosomal STR loci, one insertion/deletion polymorphic marker on the Y chromosome, Amelogenin and two internal quality control markers (IQCS and IQCL) using biological stains found in different crime scenes. The study investigated the performance of several tests, including: sensitivity, reproducibility, stability, heterozygote balance, precision, mixture study and concordance study. The results showed that the assay was reproducible, sensitive, accurate and robust. Sensitivity testing showed that a full profile could be obtained even with 63 pg of human DNA. Heterozygous allele balance varied between 60-99% for samples with total DNA input ranging from 1 ng-500 pg. It is also suitable for mixture studies which occur when the evidence contains a mixture of DNA coming from several contributors. All alleles of minor contributors were called for ratios of 1:1, 1:3 and 3:1. Overall, the current study demonstrates that this multiplex assay is robust and reliable as an assay for human identification with forensic casework samples, and most importantly is suitable to be used in Dubai Forensic Laboratory and other forensic laboratories worldwide. This study is the first to evaluate Virifiler™ Plus with casework samples.

Keywords: Concordance study, heterozygote balance, limit of detection, limit of quantification, mixture study, sensitivity, STRs.

Title and Abstract (in Arabic)

تفعيل بصمة وراثية تتكون من 23 موقع جيني لاستخدامها في تطبيقات الأدلة الجنائية

الملخص

تعتبر ترددات البصمة الوراثية القصيرة عبارة عن سلسلة قصيرة من القواعد النيروجينية المتكررة والتي يتراوح طولها ما بين 2-8 قواعد نيروجينية زوجية، وهي تشكل ما يقارب 3% من تكوين الحمض النووي للإنسان. أصبحت ترددات المواقع الجينية للبصمة الوراثية العلامة الجينية المختارة في التحليل الجنائي للعينات البيولوجية. وأثبتت أنها وسيلة تمييزية للكشف عن هوية الإنسان في التحاليل الجنائية. إن الهدف الرئيس من هذه الأطروحة هو تقييم فحص ترددات المواقع الجينية للبصمة الوراثية (Virifiler™ Plus) والتي تتكون من 23 موقع جيني منتشرة على الكروموسومات الرئيسية المكونة للحمض والنووي بالإضافة الى مواقع من الحمض النووي متعددة الأشكال على الكروموسومين (XY) اللذان يحددان جنس الإنسان وعلامات مراقبة جودة تحاليل البصمة الوراثية خاصة العينات المرفوعة من مسرح الجريمة. بحثت هذه الدراسة في أداء العديد من الاختبارات بما في ذلك: الحساسية، قابلية إعادة الحصول على نفس النتائج بالتكرار، الثبات، توازن الزيغوت المتغاير، الدقة، دراسة العينات المختلطة التي تنتج من الآثار المحتوية على الحمض النووي لعدة أشخاص ودراسة توافق العينات. برهنت الدراسة بأن هذا الفحص قابل لإعادة الإنتاج وعلى درجة عالية من الحساسية والدقة والقوة. هذا وأظهرت اختبارات الحساسية انه يمكن الحصول على قراءات متكاملة من الحمض النووي باستخدام كمية 63 بيكوغرام من الحمض النووي الأدمي. تراوح توازن الزيغوت المتغاير بين 60-99% للعينات التي تكون كمية الحمض النووي فيها 1 نانوجرام-500 بيكوغرام. يعتبر هذا الفحص مناسباً لدراسة العينات المختلطة. حيث أن جميع أليلات المساهم الثانوي كانت مقروءة بالنسب 1:1، 1:3، و 3:1. تظهر الدراسة، وبشكل عام، أن هذا الفحص مناسب ودقيق لتحديد هوية الإنسان في العينات المرفوعة من مسرح الحوادث الجنائية وملائم للاستخدام في المختبر الجنائي بدبي وغيرها من المختبرات الجنائية حول العالم. هذه الدراسة هي أول دراسة لتقييم (Virifiler™ Plus) واستخدامها لتحاليل البصمة الوراثية للعينات المرفوعة من مسرح الجريمة.

مفاهيم البحث الرئيسية: دراسة توافق العينات، توازن الزيغوت المتغاير، علامات مراقبة جودة تحاليل البصمة الوراثية، دراسة العينات المختلطة، الحساسية، ترددات البصمة الوراثية.

Acknowledgements

Firstly, all my prayers and thanks are due to Allah Almighty, without his well and power I could not achieve this state.

Secondly, I would like to thank special people around me, my main Supervisor Prof. Synan AbuQamar and co-supervisor Dr. Rashed Alghafri, who encouraged me and put their faith and belief in my effort, guided me and shared their experience and knowledge with me.

I'm deeply indebted to all examining committee members for their guidance, support and assistance throughout the preparation of this thesis.

Finally, special thanks go to my parents, husband, kids, brothers, and sisters who supported me along the way. I am sure they suspected it was endless. In addition, many thanks are extended to my colleagues and friends in Dubai Police who supported me in each step of my research and thesis preparation.

Dedication

To my beloved parents and family

Table of Contents

Title	i
Declaration of Original Work	ii
Copyright	iii
Advisory Committee	iv
Approval of the Master Thesis	v
Abstract	vii
Title and Abstract (in Arabic)	viii
Acknowledgements	ix
Dedication	x
Table of Contents	xi
List of Tables.....	xiii
List of Figures	xiv
List of Abbreviations.....	xv
Chapter 1: Introduction	1
1.1 Literature Review	1
1.1.1 History of Forensic DNA.....	1
1.1.2 DNA Typing Methods	2
1.1.3 Type of STRs	2
1.1.4 Trace DNA Definition	5
1.1.5 DNA Inhibitors	6
1.1.6 DNA Database	8
1.1.7 Six-dye STR Kits	8
1.2 Statement of the Problem.....	10
1.3 Hypothesis and Objectives	10
Chapter 2: Methods	11
2.1 Research Design	11
2.1.1 Human DNA Samples.....	11
2.1.2 Pre PCR Sample Preparation	11
2.2 PCR Amplification and Thermal Cycling Conditions.....	14
2.3 Capillary Electrophoresis (CE).....	14
Chapter 3: Results	16
3.1 Sensitivity Experiments and Determination of Thresholds	16

3.2 Heterozygote Balance (HB).....	21
3.3 Reproducibility	24
3.4 Allele Call Accuracy and Size Precision	25
3.5 DNA Mixture Study	34
3.6 Stability Study	35
3.7 Success Rate and Concordance	36
3.8 Casework Samples.....	37
Chapter 4: Discussion	49
Chapter 5: Conclusion.....	51
References	52
Appendix	55

List of Tables

Table 1: Amount of sample needed for PCR reaction	13
Table 2: Thermo cycler program for the assay	14
Table 3: Illustration of allele dropout in template DNA input ranging from 1000-8 pg	18
Table 4: Analytical threshold (AT) calculated from negative control samples.....	19
Table 5: Analytical threshold (AT) calculated from sensitivity study.....	20
Table 6: Stochastic threshold (ST) calculation	21
Table 7: T-test comparing HB between 16 pg and 500 pg DNA input.....	24
Table 8: Allele call of control DNA 007 replicates	25
Table 9: ANOVA test comparing 11 allelic ladders (AL) from one instrument	32
Table 10: ANOVA test comparing 34 allelic ladders (AL) from 2 instruments	33
Table 11: Mixture study	34
Table 12: Different casework samples used to assess the multiplex assay.....	38
Table 13: Volume of each diluted DNA sample required to prepare mixture set 1	55
Table 14: Volume of each diluted DNA sample required to prepare mixture set 2	55
Table 15: Concordance study with SRM 2391c samples (component A, B and C).....	56
Table 16: Concordance study with blood and buccal swab samples using GlobalFiler (GF) and Verifiler Plus (VFP) PCR kits	58

List of Figures

Figure 1: Percentage of allele call detected in sensitivity test of template DNA 007 ranging from 1000-8 pg, n = 27	16
Figure 2: Average peak height of control DNA 007 ranging from 1000-8 pg in sensitivity test, n = 27	17
Figure 4: Heterozygote balance average in all dye channels	23
Figure 5: Average SD of allele size in each marker, n= 34	26
Figure 6: Sizing precision testing of allelic ladder across 12 injections, n= 34	26
Figure 7: Allele range and detection size precision for each marker in the blue dye	27
Figure 8: Allele range and detection size precision for each marker in the green dye	28
Figure 9: Allele range and detection size precision for each marker in the yellow dye	29
Figure 10: Allele range and detection size precision for each marker in the red dye	30
Figure 11: Allele range and detection size precision for each marker in the purple dye	31
Figure 12: The effect of hematin porcine 0.6 mM on allele detection of DNA control 007	35
Figure 13: The effect of humic acid on allele detection of DNA control 007	36
Figure 14: Electropherogram of DNA control 007 with 500 pg	39
Figure 15: Electropherogram of a cigarette butt sample (1000 pg)	41
Figure 16: Electropherogram of a swab of bottle (30 pg) using two PCR assays	43
Figure 17: Illustration of two internal quality control sensors	44
Figure 18: Interpretation of the sample in the presence of IQC	44
Figure 19: Electropherogram of bone sample (500 pg)	45
Figure 20: Electropherogram of blood sample (1400 pg)	47

List of Abbreviations

AT	Analytical threshold
AL	Allelic ladder
bp	Base pair
CE	Capillary electrophoresis
CODIS	Combined DNA index system
LOD	Limit of detection
LOQ	Limit of quantification
nt	Nucleotide
PCR	Polymerase chain reaction
PHR	Peak height ratio
RFLP	Restriction fragment length polymorphism
RFU	Relative fluorescence unit
STR	Short tandem repeats
VNTR	Variable number of tandem repeats

Chapter 1: Introduction

1.1 Literature Review

Advanced molecular biological tools are universally used in DNA analysis to identify information contained in crime scene evidence. These advances have allowed scientists to provide critical information to solve crimes and the criminal justice community to convict the guilty and justify the innocent. Scientific research continues to develop new automated technologies and methods to yield more information from limited samples allowing scientists to optimize time and effort [1].

1.1.1 History of Forensic DNA

In 1980s, forensic scientist used statistical interpretation to analyze the biological stains from different type of cases such as homicide and sexual assault that could represent only 10% of the population; Unfortunately, results were not accurate as it ruled out 90% of the population as a possible donor [1].

In 1985, Alec Jefferys discovered a new method to analyze biological stains called DNA typing. It was found that certain regions of DNA contain specific sequences that are next to each other and repeated a number of times. These regions are known as variable number of tandem repeats (VNTR). He also proved the ability of these repeats to differentiate human individuals. Moreover, a technique by Jefferys was developed to examine the length variation of these sequence repeats called restriction fragment length polymorphism (RFLP) analysis. This technique uses multi locus probe and a restriction enzyme that cuts the region of DNA surrounding the VNTRs [2].

Since that time, DNA typing methods has been used in human identity testing in forensic laboratories. Enormous growth has been seen in the use of DNA evidence in crime scene investigation and paternity testing. More than 150 public forensic laboratories and other private paternity testing laboratories are conducting thousands of DNA tests in the United States [2] and in other forensic laboratories around the world.

1.1.2 DNA Typing Methods

STR markers analyzed by capillary electrophoresis (CE) represent the gold-standard for forensic DNA analysis. For the past twenty years, STR loci from the human genome have been the genetic markers of choice in forensic DNA analysis in large measure. This is because the multi-allelic nature of STRs produce many possible genotype combinations that can aid human identification and most importantly DNA mixture interpretation. STRs are copied by polymerase chain reaction (PCR) and the analysis is performed by size-based DNA separations using capillary electrophoresis or CE. However, analysis of PCR product length alone fails to capture the potential internal sequence variation that may exist in many STR loci detected via base composition mass spectrometry or through full sequence analysis [3].

1.1.3 Type of STRs

STR loci can vary in three manners: the repeat unit length (e.g., di-, tri-, tetra-penta-, hexa-nucleotides), the number of repeat units (e.g.10–25 repeats) and in the rigor with which alleles conform to an incremental repeat pattern. In one of the early studies by the UK Forensic Science Service (FSS), STR loci were categorized as simple, compound or complex based on how well alleles conformed to the core repeat pattern [3].

Simple repeats, such as TH01 with an AATG repeat motif, contain repeat units of identical length and sequence, although they may occasionally have non-consensus repeats like the TH01 9.3 allele with a [AATG] 6 ATG[AATG] 3 sequence [3].

Compound repeats comprise two or more adjacent simple repeats, such as TCTA and TCTG in the tetranucleotide STR locus vWA. Complex repeats may contain several repeat blocks of variable unit length as well as variable intervening sequences with numerous variant alleles, such as the STR loci D21S11 or FGA. Some STR alleles contain partial repeats (e.g., the ATG interspersed between AATG repeats in the TH01 9.3 allele) or other sequence variation that has arisen due to mutation in the repeat region or in the nearby flanking regions [3].

Nomenclature for the designation of length-based STR alleles has been developed over the years by the DNA Commission of the International Society for Forensic Genetics (ISFG) and categorized under simple repeat, variant allele, compound repeat and complex repeat [3]. With simple repeats, the number of repeat units is counted (e.g., TH01 allele 7). While variant alleles are designated by counting the number of full repeats, adding a decimal point, and then counting the number of nucleotides (nt) in the incomplete repeat (e.g., TH01 allele 9.3 with nine full repeats plus three additional nt). For compound repeats, alleles are designated by counting the total number of full repeats (e.g., vWA allele 18 comprised of 1 TCTA + 4 TCTG + 13 TCTA repeats). With complex repeat systems, the typical approach taken is to establish a mathematical relationship to the (nt length of a consensus allele (e.g., D21S11 allele 27). For highly variable systems such as SE33, alleles may be identified according to their relative size compared to an allelic ladder containing sequenced alleles, even though it is understood that internal sequence variation is possible [3].

DNA typing of STRs located in the human genome has proven to be an extremely discriminating method for human identification in forensic and paternity applications for decades. It has been widely used for the identification of individuals based on their DNA characteristics [4]. In forensic applications, STR sequence data is expected to increase the effective number of alleles, which may aid mixture interpretation in some cases. More generally, this type of data has shown benefits in characterizing STR mutation rates which contributes to our foundational understanding of these loci [3]. Expansion to additional STRs while retaining connection to legacy STR profile information appears to be the way forward in the United States and Europe [5].

Single nucleotide polymorphism (SNP) can overcome the technical difficulties with the forensic use of STRs. The use of short PCR amplicons (50 nt or less) leads to a successful analysis of low amounts of highly degraded DNA, which is difficult with highly polymorphic STRs because of their repetitive sequence [6]. Furthermore, owing to the very short amplicons that can be employed in SNPs, successful SNP profiling can be obtained from degraded DNA which STR profile cannot be obtained. SNP profiling lacks artefacts that appears in STR profiles and complicates the interpretation of results specially with low amount of DNA [6]. However, challenges are also exist with the use of autosomal SNPs for human individual identification in forensic investigations. Because SNPs are bi-allelic and less polymorphic that multi allelic STRs, they are less informative in the analysis of mixtures of DNA from multiple individuals. Therefore, using higher number of SNPs may help, but the use of tri-allelic SNPs, combined with multiplex genotyping technologies may compensate for this effect [6].

Another forensic approach is using Y-STRs for male identification in mixed stain analysis. Since 1990, haplotypes from sets of male specific Y-STRs have been used for male identification [6]. The new DNA markers promise to improve human identification with the ability to identify two or more male individuals in cases of sexual assault. When male contributors are not shown in autosomal STR profiles as a result of preferential PCR amplification of the excess female contributor [6].

Several studies confirmed that Y-STR analysis plays an important role in different type of cases such as the analysis of: complex mixtures, sexual cases having samples with no spermatozoa [7], samples with multiple contributor mixtures, and mixture samples which shows no male component [8]. Commercial kits have been improved over years, and more Y- STR multiplexes have been developed [9] which provides rich information to be used in constructing phylogenetic trees and the deduction of ethnic origin [10].

1.1.4 Trace DNA Definition

It is important to understand what is exactly meant by the term trace DNA. Nowadays, trace DNA collected from crime scene has become a large part of the average forensic laboratories' workload. Remarkably low DNA amounts (<100 pg) have been successfully analyzed to obtain profiles from a wide range of sample types. Touched objects constitute the most common source of trace DNA, but any type of biological material present in low amounts may be considered as trace, including minute blood deposits and saliva residue on partially consumed food. In addition to supplementing existing analysis techniques in serious crime cases, trace DNA can allow investigation of volume crime cases such as burglary, vehicle theft and run over, where DNA evidence had not previously been considered usable. However, despite

the widespread use of trace DNA, at present there are very few specific validated methods. This has led to controversy in the use of trace DNA, and particularly the low copy number amplification technique. It has been established that the use of existing methodology that specifically developed for high-copy number samples, leads to significant levels of artefacts with trace DNA, including allele drop-out and drop-in, stutter, and allelic/locus imbalance. To minimize these artefacts, there are numerous modifications that can be made to existing methods to increase the success of trace DNA analysis. These include reduced extraction volumes, increased cycle number, reduced PCR volume, and increased injection time for CE [1].

Recent researches have introduced techniques such as post-PCR purification, whole genome amplification and molecular crowding which can increase success rates with trace DNA significantly. Moreover, each step starts from sample collection, extraction, amplification and fragment detection that can be optimized to trace DNA. Indeed, the use of trace DNA analysis techniques with high sensitivity must bring an increasing awareness of the potential for contamination, both within the laboratory and at crime scenes, especially with DNA traces from cold cases, which were not collected or stored with highly sensitive DNA detection techniques. Although trace DNA continues to be used within forensic biology, a wide range of practices may need to be modified to ensure accuracy and reliability [1].

1.1.5 DNA Inhibitors

The most common cause of PCR failure is the presence of PCR inhibitors in the samples, especially when dealing with adequate copies of DNA. It causes a great challenge for scientist analyzing biological remains recovered from the environment. Casework samples are in a high risk of containing different type of PCR inhibitory

compounds which interfere with downstream DNA typing success, resulting in imbalanced, partial or negative DNA profiles. Theoretically, the activity of the inhibitors may affect every component of PCR reaction including binding to the template DNA, the nt, the amplification primers, Mg^{2+} and the Taq polymerase [11].

Degree of inhibition could have different effect, severe inhibition can lead to the loss of alleles from the larger STR loci, or complete false-negative results, which is a pattern similar to severe template degradation that can mistakenly attributed. While a slight to moderate inhibition which can result in a minor loss of alleles and misestimating of the affected sample's DNA quantity, it has potential consequences for downstream applications such as STR analysis. Generally, only larger loci are lost when the Taq is affected by the inhibitors. However, alleles may be lost regardless of amplicon size when inhibitors bind the DNA, based on where in the template the inhibitor binds [12, 13].

PCR inhibitors associated with casework samples could be humic acid in soil, hematin in red blood cells, humic substances in soil, melanin in hair and skin, myoglobin in tissue, bile salts and complex polysaccharides in feces, collagen in soft tissue and bone, polysaccharides in plants [13, 14]. Moreover, STR typing is limited by the quality of human DNA obtained from forensic casework samples that can be influenced by environmental factors which may cause different degrees of degradation, that have a negative impact on the amplification process especially of STR systems with large amplicons [15]. Amplifying of mini STRs, which provides shorter length markers, in addition of increasing the amount of classical STRs marker showed obtaining more reliable results [11].

1.1.6 DNA Database

Forensic scientists have become able to identify individuals with a significant discrimination power by combining DNA profiling results at several independent STR loci. The STR technology is more powerful with the establishment of centralized forensic DNA databases in many countries around the world. This is because it provides valuable information for direct matching of DNA profiles of individuals to those of DNA samples collected at crime scenes. After nearly three decades of operation, the size of the centralized DNA database continues to grow [12]. In order to reduce the number of adventitious matches and to increase international compatibility as well as the power of discrimination for criminal and missing person cases, the Federal Bureau of Investigation (FBI) expanded the combined DNA Index system (CODIS) core loci from the existing 13 to 20 [5].

1.1.7 Six-dye STR Kits

In 2012, a group of scientists started the first beta-testing with a six-dye STR kit prototype containing 24 loci (GlobalFiler™ PCR Amplification Kit) developed by Life Technologies in response to the CODIS Core Loci Working Group's recommendation to expand the CODIS Core Loci; followed by a validation study of these 24 markers in 2014 [16]. Investigator1 24plex QS Kit and Investigator1 24plex GO! Kit are other examples of six-dye STR kit containing 24 loci, developed by QIAGEN [17]. Another group of scientists proved that with the advancement of the six-dye chemistry, it is now possible to expand the number of STR systems analyzed within a single reaction, by examining the performance of another six-dye, multiplex containing 27 loci the (PowerPlex1 Fusion 6C System) developed by Promega [18].

It is worth mentioning that the six-dye kits allow analyses of a larger volume of input DNA (*i.e.*, 15 μ L instead of 10 μ L). The fact that they possess 8-10 mini-STR systems with amplicon sizes of less than 220 bp further improves their information recovery from heavily degraded samples [19].

In this study, an evaluation of a six-dye STR multiplex assay (VeriFiler™ Plus) was conducted; this assay is composed of the following markers:

- 23 autosomal STR loci (D3S1358, vWA, D16S539, CSF1PO, TPOX, D8S1179, D21S11, D18S51, D2S441, D19S433, TH01, FGA, D22S1045, D5S818, D13S317, D7S820, D10S1248, D1S1656, D12S391, D2S1338, D6S1043, Penta D, Penta E).
- 1 insertion/deletion polymorphic marker on the Y chromosome (Y indel) and Amelogenin (sex-determining marker)
- 2 internal Quality control markers (IQCL & IQCS)

Evaluation of the assay with casework samples was performed using a 3500 genetic analyzer to detect the different fragment size of alleles. This study included the analysis of different parameters and aspects; sensitivity study to determine the lowest amount of DNA required to produce a complete electropherogram, determination of analytical threshold which is the lowest relative fluorescence units (RFU) value at which DNA can be distinguished from noise, determination of stochastic threshold which is the threshold at which the analyst can be confident that if one peak for a heterozygote is above this threshold, then its sister allele will be present and should be above the analytical threshold, heterozygous balance which is the relative ratio of two alleles at a given locus, determined by dividing the peak height of an allele with a lower RFU value by the peak height of an allele with a higher RFU value, precision

and accuracy, reproducibility study is being able to obtain the same result under the same condition, genotype concordance is also conducted to assess the success rate of the assay, DNA mixtures studies is conducted to define and mimic the range of detectable mixture ratios, including detection of major and minor components, and stability study to assess the tolerance and the robustness of the assay in the presence of common type of inhibitors that could bear in casework samples.

1.2 Statement of the Problem

DNA samples collected from a crime scene showed to be the key element in solving crimes. However, the traces of DNA samples could be affected by the environmental factors which may lead to the loss of the evidence. This study aimed to evaluate the use of Verifiler™ Plus, a six-dye multiplex assay, with casework samples. This study will be beneficial for DNA forensic laboratories in UAE as well as other laboratories, since it enhances the success rate of obtaining positive results from challenging forensic samples.

1.3 Hypothesis and Objectives

This research study hypothesize that if Verifiler™ Plus is used with casework samples, success rate of obtaining positive results will increase.

The objectives of this study are:

- To measure the sensitivity, precision, accuracy and reproducibility of the Verifiler™ Plus assay,
- To study mixture sensitivity and inhibition resistance, and
- To perform a concordance study between GlobalFiler and this assay.

Chapter 2: Methods

2.1 Research Design

2.1.1 Human DNA Samples

- AmpFLSTR™ Control DNA 007 sourced from Thermo Fisher Scientific (South San Francisco, CA), and set of three control DNA SRM 2391c purchased from National institute of standard techniques (NIST).
- A set of 32 consented samples, 16 blood samples and 16 buccal swabs was prepared. Samples were extracted using PrepFiler™ Express Forensic DNA Extraction Kit (Thermo Fisher Scientific) and the AutoMate Express™ Nucleic Acid Extraction System (Thermo Fisher Scientific). The DNA was quantified using the Quantifiler™ Human DNA Quantification Kit on an Applied Biosystems™ 7500 Real-Time PCR System (Thermo Fisher Scientific).
- Pre-extracted casework samples, previously analyzed using GlobalFiler™ PCR Amplification Kit were used.

2.1.2 Pre PCR Sample Preparation

2.1.2.1 Sensitivity Experiments and Determination of Stochastic Thresholds

A serial dilution of Control DNA 007 (Thermo Fisher Scientific, South San Francisco, CA, USA) was amplified using the six-dye multiplex assay (Verifiler™ Plus). Four replicate reactions were performed and analyzed with the following inputs: 1000, 750, 500, 250, 125, 63, 32, 16 and 8 pg DNA. Non-template controls (NTCs) were run. Amplified product was electrophoresed on the 3500 instrument and analyzed with GeneMapper™ ID-X 1.4 software. 11 PCR negative controls from multiple

injections were analyzed across the six channels in the range 60–450 base pairs to determine the analytical threshold.

2.1.2.2 Peak Height Ratio

Data from sensitivity study was used to calculate the heterozygote balance (HB) in each dye individually and then all together.

2.1.2.3 Reproducibility and Allele Call Accuracy

A total of 34 allelic ladder from two different instruments across multiple injections were analyzed, and the average base pair (bp) size and standard deviation (SD) of each allele in the allelic ladder was calculated.

2.1.2.4 DNA Mixture Study

DNA mixtures was prepared using two male DNA control provided with standard SRM 2391c (component B and C) in ratios of 1:1, 3:1, 7:1, 10:1, 15:1 and vice versa. Mixtures were amplified in triplicate. Electrophoreses was performed for the amplified product on the 3500 instrument and analyzed with GeneMapper™ ID-X 1.4 software.

2.1.2.5 Stability Study

Hematin porcine (Sigma) was prepared at a concentration of 0.6 mM and added to the PCR component in the following amount: 1µl, 1.5 µl, 3.125 µl, 6.25 µl, 9.5 µl and 12.5 µl. Humic acid (Sigma) was dissolve in water at a concentration of: 200 ng/µl, 150 ng/µl, 100 ng/µl, 80 ng/µl, 60 ng/µl. Test was performed in triplicates.

2.1.2.6 Concordance Study

Standard Reference material SRM-2391c derived from 2 single male donor and 1 female donor (component A, B and C) produced and certified by the National Institute of Standards and Technology (MD, USA) were amplified, and allele calls were analyzed against the certified STR allele values. A total of 32 consented samples (Ref: DPSC-2019-EA-018), 16 blood samples and 16 buccal swabs were amplified, and allele calls were analyzed against profiles from the same set of samples previously analyzed using GlobalFiler™ Amplification kit.

2.1.2.7 Casework Samples

A total of 8 bone samples (Bn), 7 swabs of bottle (Bt), 5 cigarette butts (CB), 1 plug, 1 blood from the floor along with a human tissue sample (Ref: DPSC-2019-EA-018), previously analyzed using GlobalFiler™ Amplification kit, were used to test the applicability of the multiplex on casework samples. Controls were amplified along with casework samples; amplification reaction was performed with final concentrations mentioned in Table 1. PCR was programmed as recommended by manufacturer.

Table 1: Amount of sample needed for PCR reaction

Sample	Add
Negative control	17.5 µL of nuclease-free water
Test Sample	17.5 µL of DNA (500 pg)
Positive control	Combined, then added to the reaction tube: <ul style="list-style-type: none"> • 5 µL of DNA Control 007 (0.1 ng/µL) • 12.5 µL of nuclease-free water
Master Mix	5.0 µL
Primer set	2.5 µL

2.2 PCR Amplification and Thermal Cycling Conditions

The Master Mix and Primer Set were vortexed for 3 seconds and the tubes were centrifuged briefly. Total of 5.0 μ L of Master Mix and 2.5 μ L of Primer set per sample were pipetted into 1.5 ml tube and the reaction mixture was vortexed for 3 seconds, then centrifuged briefly and 7.5 μ L of reaction mixture was dispensed into each MicroAmp™ tube. Samples were prepared and added to the appropriate tube (the final reaction volume is 25 μ L). The sample input amount volume was adjusted as needed to reach DNA input amount of 500 pg. The solution was mixed until it was homogenous and each tube was centrifuged at 3,000 rpm for approximately 30 seconds in a tabletop centrifuge.

The thermal cycling conditions was programmed as recommended by manufacturer (Table 2). Sample tubes were loaded into the thermal cycler, the heated cover was closed, then the run was started.

Table 2: Thermo cycler program for the assay

Initial incubation	First stage (2cycles)	Second stage (27 cycles)		Final extension	Final hold	
	Denature	Anneal/ extend	Denature	Anneal/ extend		
Hold	Cycle (29 Cycle)				Hold	Hold
95°C	96°C	62°C	96°C	59°C	60°C	4°C
1 min	10 sec	90 sec	10 sec	90 sec	5 min	∞

2.3 Capillary Electrophoresis (CE)

9.5 μ L of Hi-Di™ Formamide, 0.5 μ L of GeneScan™-600 LIZ size standard (both from Life Technologies) and 1 μ L of amplified sample was added into each well. Samples were denatured for 3 min at 95° C. CE was performed on the 3500 (8-

capillary) genetic analyzer (Life Technologies). Data were collected using the 3500 Data Collection Software v.2.0 and HID files generated with the 3500 Data Collection Software v.2.0 was analysed using GeneMapper1 ID-X Software v1.4.

Chapter 3: Results

3.1 Sensitivity Experiments and Determination of Thresholds

Scientists conduct sensitivity tests for number of reasons including the need to determine the lowest amount of DNA required to produce a complete electropherogram. Different amount of control DNA 007 (Thermo Fisher Scientific) was used for sensitivity study.

To assess this test the percentage of allele call was calculated. Full STR profiles (100% of allele call) were obtained from control DNA 007 (Thermo Fisher Scientific) samples ranging from 1000 pg down to 63 pg (Figure 1), and drop out was detected starting from 32 pg recovering 95% of expected alleles.

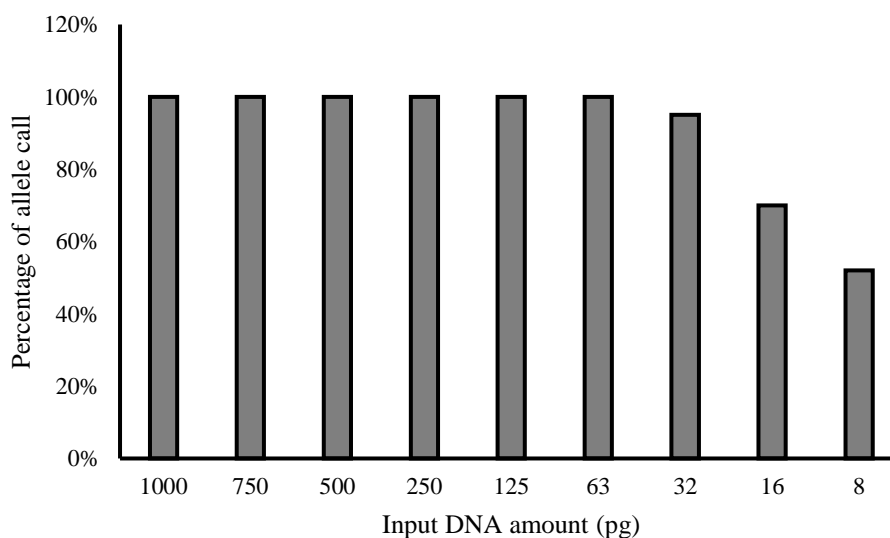


Figure 1: Percentage of allele call detected in sensitivity test of template DNA 007 ranging from 1000-8 pg, n = 27

Figure 1 illustrates the percentage of allele call resulted from the following DNA input of control DNA 007: 1000, 750, 500, 250, 125, 63, 32, 16 and 8 pg. 70% and 52% of all expected alleles were recovered at 16 pg and 8 pg respectively.

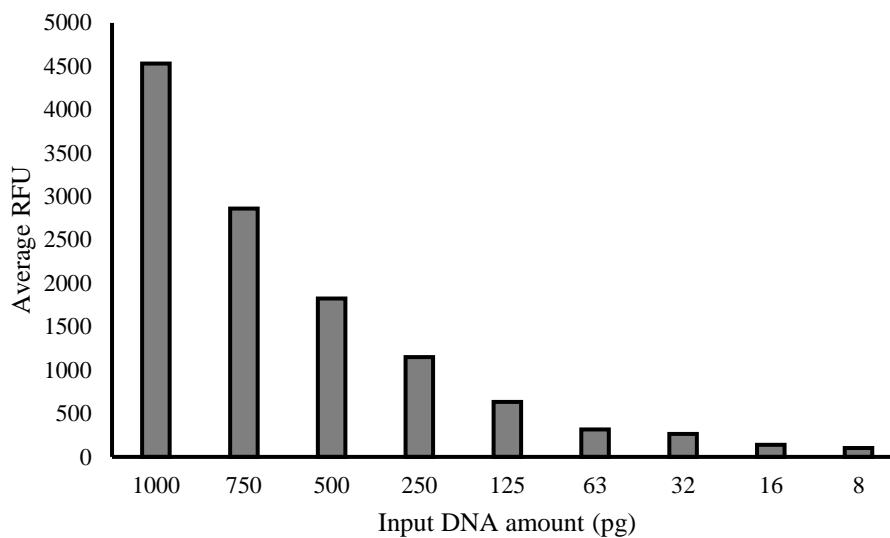


Figure 2: Average peak height of control DNA 007 ranging from 1000-8 pg in sensitivity test, n = 27

Overall, as the DNA input decrease, the average peak height of the alleles also decrease (Figure 2); indicating decrease of the quality and the completeness of the profiles. This result shows well correlation between the signal height and the serially diluted template DNA.

Table 3: Illustration of allele dropout in template DNA input ranging from 1000-8 pg

Marker	DNA Template Amount								
	1000 pg	750 pg	500 pg	250 pg	125 pg	63 pg	32 pg	16pg	8pg
D3S1358	Green	Green	Green	Green	Green	Green	Yellow	Green	Green
vWA	Green	Green	Green	Green	Green	Green	Green	Green	Yellow
D16S539	Green	Green	Green	Green	Green	Green	Green	Green	Green
CSF1PO	Green	Green	Green	Green	Green	Green	Green	Yellow	Yellow
D6S1043	Green	Green	Green	Green	Green	Green	Green	Yellow	Yellow
Yindel	Green	Green	Green	Green	Green	Green	Green	Green	Green
AMEL	Green	Green	Green	Green	Green	Green	Green	Green	Green
D8S1179	Green	Green	Green	Green	Green	Green	Yellow	Green	Yellow
D21S11	Green	Green	Green	Green	Green	Green	Green	Green	Green
D18S51	Green	Green	Green	Green	Green	Green	Green	Yellow	Green
D5S818	Green	Green	Green	Green	Green	Green	Green	Yellow	Green
D2S441	Green	Green	Green	Green	Green	Green	Green	Yellow	Yellow
D19S433	Green	Green	Green	Green	Green	Green	Green	Green	Yellow
FGA	Green	Green	Green	Green	Green	Green	Green	Green	Yellow
D10S1248	Green	Green	Green	Green	Green	Green	Green	Yellow	Green
D22S1045	Green	Green	Green	Green	Green	Green	Green	Green	Green
D1S1656	Green	Green	Green	Green	Green	Green	Green	Green	Yellow
D13S317	Green	Green	Green	Green	Green	Green	Green	Green	Green
D7S820	Green	Green	Green	Green	Green	Green	Green	Green	Yellow
Penta E	Green	Green	Green	Green	Green	Green	Green	Green	Green
Penta D	Green	Green	Green	Green	Green	Green	Green	Green	Yellow
TH01	Green	Green	Green	Green	Green	Green	Green	Green	Yellow
D12S391	Green	Green	Green	Green	Green	Green	Green	Yellow	Green
D2S1338	Green	Green	Green	Green	Green	Green	Green	Green	Green
TPOX	Green	Green	Green	Green	Green	Green	Green	Green	Green

Note: Green wells represent full allele call, yellow wells represent allele drop out.

The number of dropouts increase with decreasing the input amount of DNA (Table 3). Profiles generated from 32 pg of DNA input showed two allele dropouts, detected in D3S1358 (Blue Dye) and D8S1179 (Green Dye). For 16 pg of DNA input, allele dropout was detected in the Blue Dye (CSF1PO, D6S1043), Green Dye (D18S51, D5S818), Yellow Dye (D2S441, D10S1248) and in the Purple Dye (D12S391). Total of 11 allele dropout was detected in the 5 dyes of profiles generated from 8 pg DNA template (Table 3). No locus dropout was detected. A number of pull up peaks was also detected in samples with DNA input > 500 pg, and were clearly

distinguishable from the true allele peaks, which points to the optimum range to be determined at 125 - 500 pg. All the alleles in those profiles remained balanced and was not affected with the pull up peaks.

Analytical threshold (AT) is the minimum height requirement, above which detected peaks can be reliably distinguished from background noise; peaks above this threshold are generally not considered noise and are either artifacts or true alleles. It was calculated using the following formula: $AT = 2 \times (\text{Max. PH} - \text{Min. PH})$ [22]. To calculate AT two different set of samples were used to calculate an accurate AT for casework samples.

The first set is composed of 11 negative controls from multiple injections, where the analysis of baseline noise was conducted, and the AT calculated from these set was (36.8 RFU) (Table 4) which is considered to be very low AT and might cause an increase in the baseline noise if a mass of DNA amount (>1 ng) was amplified. A lot of pull ups to be called specially with strong DNA input samples. However this low threshold can be useful with casework samples of low DNA amount.

Table 4: Analytical threshold (AT) calculated from negative control samples

Dye	Max. PH	Min. PH	AT= 2 * (Max. PH – Min. PH),	Average AT
blue	19	2	34	36.8
Green	20	4	32	
yellow	26	1	50	
red	17	2	30	
Purple	22	3	38	

Max. PH: Maximum peak height; Min. PH: Minimum peak height

The second set composed of positive control samples from sensitivity study. Calls for all true alleles and artefacts were removed, and the minimum and maximum peak height of the identified baseline noise was calculated in each dye channel. The average AT for all dyes is 76.8 RFU (Table 5), so the overall analytical threshold was set to 80 RFU.

Table 5: Analytical threshold (AT) calculated from sensitivity study

Dye	Max. PH	Min. PH	AT= 2 * (Max. PH – Min. PH)	Average AT
Blue	30	1	58	76.8
Green	33	3	60	
Yellow	37	2	70	
Red	60	3	114	
Purple	45	4	82	

Max. PH: Maximum peak height; Min. PH: Minimum peak height

The stochastic threshold (ST) is the threshold at which the analyst can be confident that if one peak for a heterozygote is above this threshold, then its sister allele will be present and should be above the analytical threshold; it is the peak height value above which it is reasonable to assume that, at a given locus, allelic dropout of a sister allele has not occurred. This can be described as the limit of quantification (LOQ). The stochastic threshold was calculated using the following formula: Average peak height + (3 x SD). It was calculated by examining the peak height of heterozygote loci where one sister allele has dropped below the analytical threshold. The highest peak height recorded was 179 RFU and the overall stochastic threshold was set to 180 RFU (Table 6).

Table 6: Stochastic threshold (ST) calculation

Average in all dye channel	SD	ST= Average Peak Height + (3* SD)	ST
113.5	22.14	179.9	180

SD: Standard deviation.

3.2 Heterozygote Balance (HB)

The HB is the relative ratio of two alleles at a given locus, as determined by dividing the peak height of an allele with a lower RFU value by the peak height of an allele with a higher RFU value, and then multiplying this value by 100 to express the PHR as a percentage. HB is used as an indication of which alleles may be heterozygous pairs and also in mixture deconvolution.

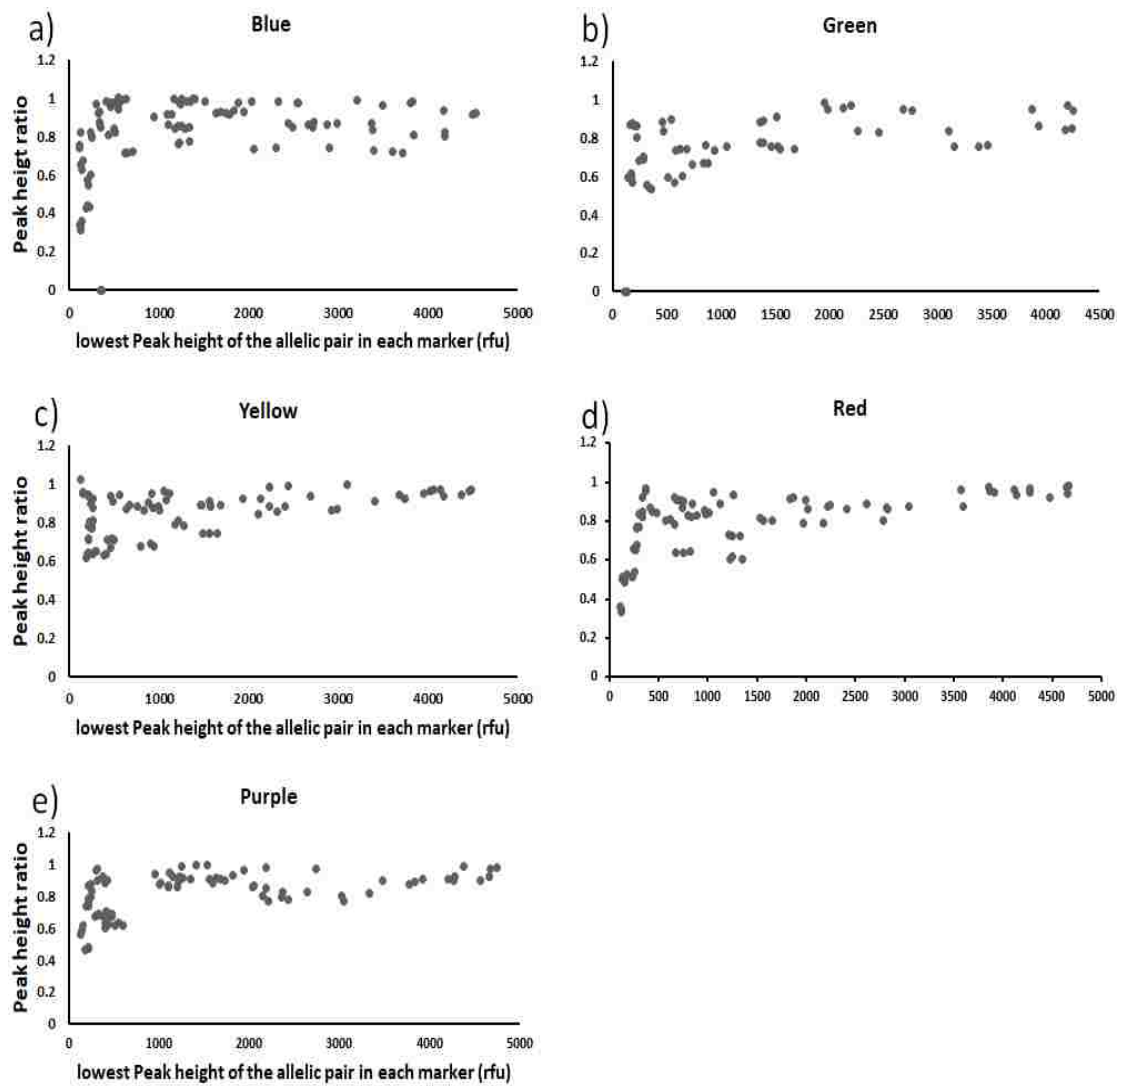


Figure 3: Peak height ratio for each dye channel observed in sensitivity study (a) blue dye channel, (b) green dye channel, (c) yellow dye channel, (d) red dye channel, (e) purple dye channel

HB was calculated individually for each dye (Figure 3). According to the recommendations of ENFSI [23, 24] the peak balance ratio of heterozygote alleles should be $> 60\%$. PHR was below 60% when the peak height of the allelic pair was lower than 250 RFU in the blue, green, red and purple dye (Figure 3 a, b, d, e) showing that heterozygous peak height ratios decreased towards lower template amounts. All the alleles recorded 60% PHR in the yellow dye (Figure 3c).

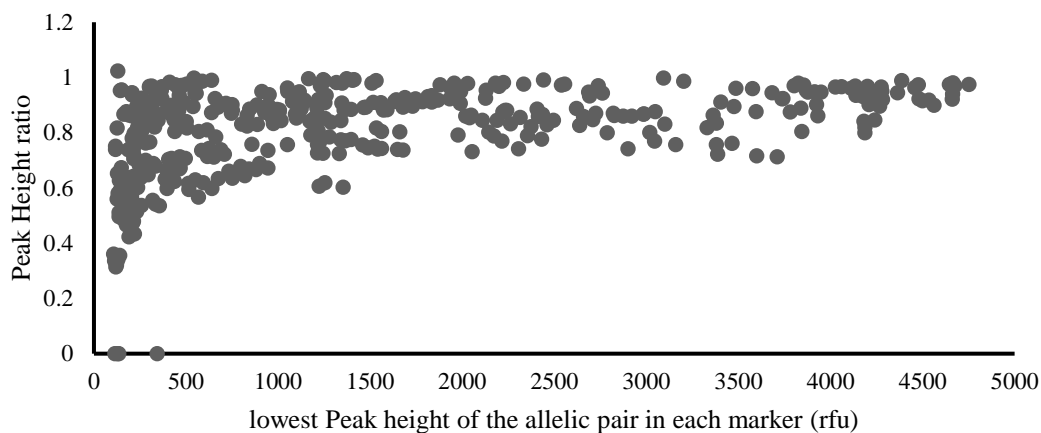


Figure 4: Heterozygote balance average in all dye channels

The overall peak height ratio in all markers is illustrated in Figure 4. The average peak height ratio varied between 99- 60% which meets the recommendation of ENFSI. Overall, HB increase toward higher allele peak heights.

Peak height ratio comparison was done between DNA profiles with 500 pg DNA input, which is considered to be the intermediate amount of DNA input, and DNA profile with 16 pg DNA input (low amount of DNA) using t-test. A p- value = $5.56343E^{-09}$ was obtained which is significantly less than α (0.05), and t-stat = 6.761035004 (Table 7). This result provides strong evidence that the amount of input DNA affects the peak height ratio balance producing lower ratios toward lower DNA input. This result might help the scientist to make correct decision about profiles generated from low template DNA samples.

Table 7: T-test comparing HB between 16 pg and 500 pg DNA input

	16 pg DNA	500 pg DNA
Mean	0.603072681	0.840966
Variance	0.03296552	0.006652
Observations	32	32
Pooled Variance	0.019808752	
Hypothesized Mean Difference	0	
df	62	
t Stat	-6.761035004	
P(T<=t) one-tail	2.78172E-09	
t Critical one-tail	1.669804163	
P(T<=t) two-tail	5.56343E-09	
t Critical two-tail	1.998971517	

3.3 Reproducibility

Reproducibility is the test of being able to obtain the same result under the same condition. To test for reproducibility of genotyping results across different sites and instruments, 500 pg as input DNA (Table 8) of Control DNA 007 was amplified in 6 replicates, and the amplified product was analyzed at two sites.

Table 8: Allele call of control DNA 007 replicates

Marker	Allele call of each sample					
	site A			site B		
	1 st injection	2 nd injection	3 rd injection	4 th injection	5 th injection	6 th injection
D3S1358	15,16	15,16	15,16	15,16	15,16	15,16
vWA	14,16	14,16	14,16	14,16	14,16	14,16
D16S539	9,10	9,10	9,10	9,10	9,10	9,10
CSF1PO	11,12	11,12	11,12	11,12	11,12	11,12
D6S1043	12,14	12,14	12,14	12,14	12,14	12,14
Yindel	2	2	2	2	2	2
AMEL	XY	XY	XY	XY	XY	XY
D8S1179	12,13	12,13	12,13	12,13	12,13	12,13
D21S11	28,31	28,31	28,31	28,31	28,31	28,31
D18S51	12,15	12,15	12,15	12,15	12,15	12,15
D5S818	11	11	11	11	11	11
D2S441	14,15	14,15	14,15	14,15	14,15	14,15
D19S433	14,15	14,15	14,15	14,15	14,15	14,15
FGA	24,26	24,26	24,26	24,26	24,26	24,26
D10S1248	12,15	12,15	12,15	12,15	12,15	12,15
D22S1045	11,16	11,16	11,16	11,16	11,16	11,16
D1S1656	13,16	13,16	13,16	13,16	13,16	13,16
D13S317	11,11	11,11	11,11	11,11	11,11	11,11
D7S820	7,12	7,12	7,12	7,12	7,12	7,12
Penta E	7,12	7,12	7,12	7,12	7,12	7,12
Penta D	11,12	11,12	11,12	11,12	11,12	11,12
TH01	7,9.3	7,9.3	7,9.3	7,9.3	7,9.3	7,9.3
D12S391	18,19	18,19	18,19	18,19	18,19	18,19
D2S1338	20,23	20,23	20,23	20,23	20,23	20,23
TPOX	8,8	8,8	8,8	8,8	8,8	8,8

3.4 Allele Call Accuracy and Size Precision

To measure the degree of variation in each fragment size, a total of 34 replicates of allelic ladder from multiple injections was run on two 3500 Genetic analyzer instruments.

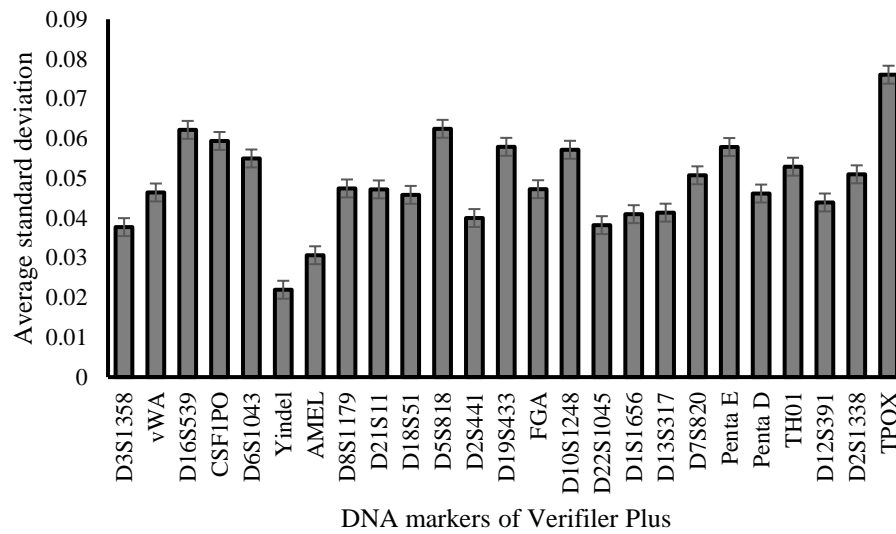


Figure 5: Average SD of allele size in each marker, n= 34

The average SD of all allele size (bp) in every loci between all replicates varied from 0.02 to 0.08 bp (Figure 5), which is within the recommended ± 0.5 bp window for genotyping as it is mentioned by ENFSI (2010) [23].

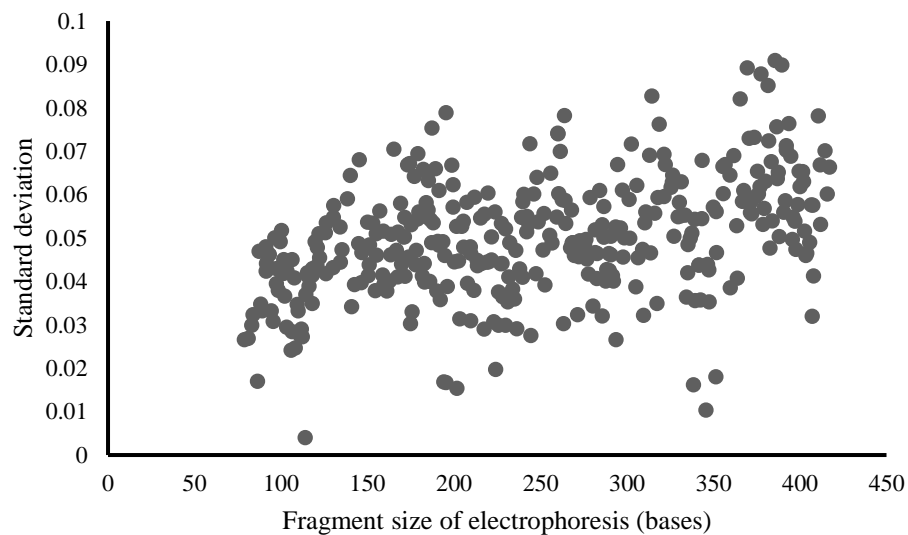


Figure 6: Sizing precision testing of allelic ladder across 12 injections, n= 34

No dropout was observed in any allelic ladder. Size variation increases with larger fragment size (Figure 6). Average length and SDs were determined for each allelic ladder fragment across all dye channels (Figures 7-11).

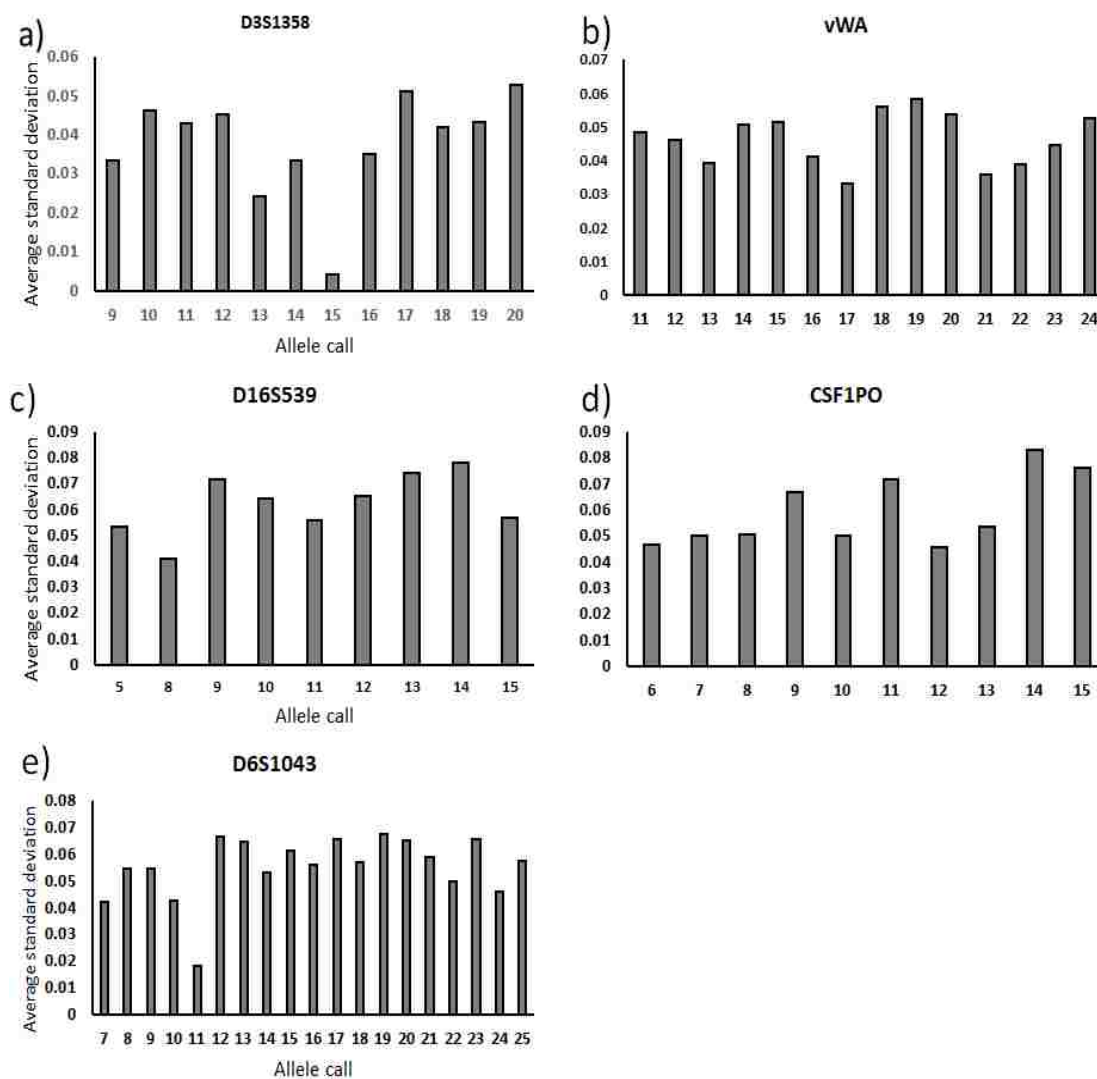


Figure 7: Allele range and detection size precision for each marker in the blue dye

Figure 7a illustrates the minimum SD which was observed for D3S1358 allele 15. While average SD of each fragment size varies between 0.02 bp to 0.08 bp among the 5 markers in the blue dye channel (Figure 7).

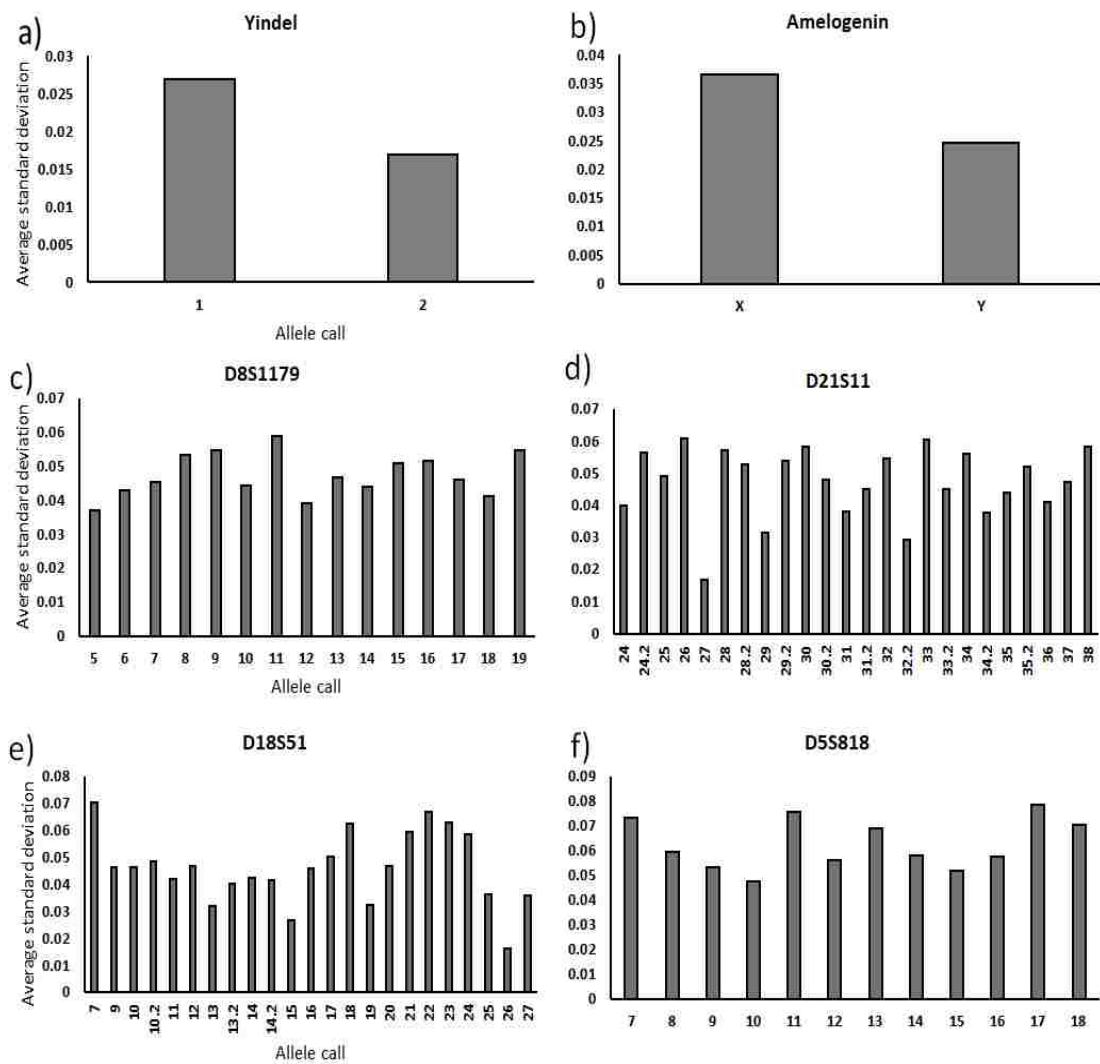


Figure 8: Allele range and detection size precision for each marker in the green dye

Figure 8 illustrates the average SD of each fragment size in 6 markers of green dye channel which varies between 0.02 bp to 0.08 bp.

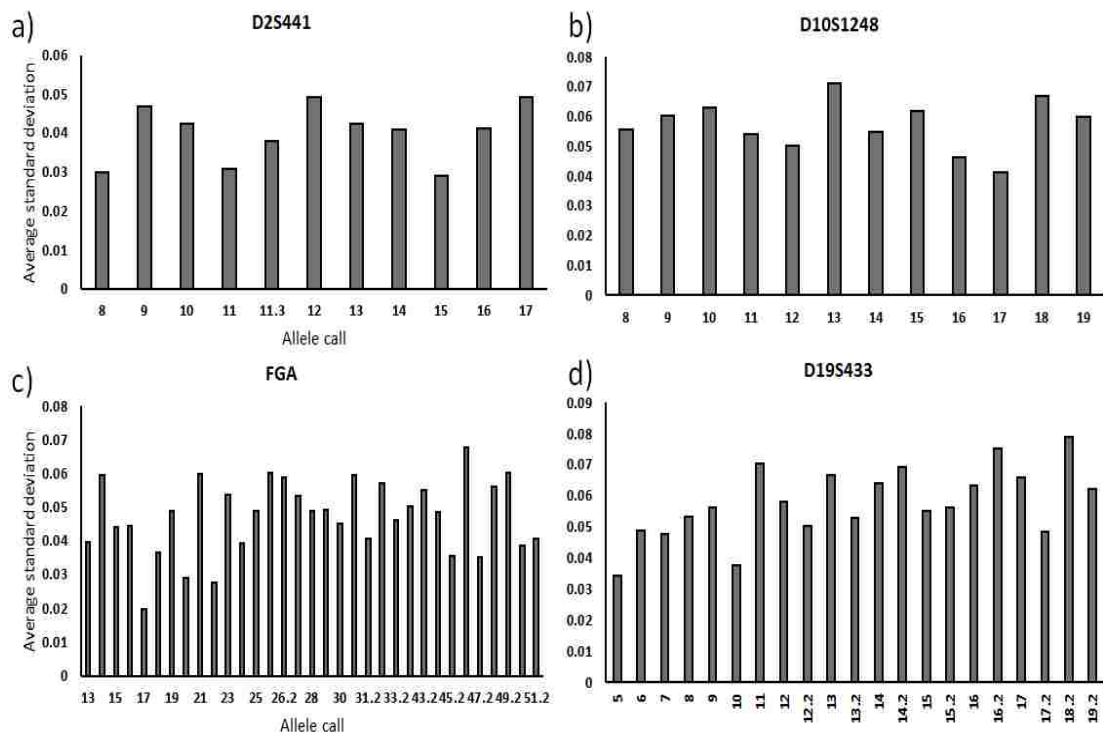


Figure 9: Allele range and detection size precision for each marker in the yellow dye

Figure 9 illustrates the average SD of each fragment size in 4 markers of yellow dye channel which varies between 0.03 bp and 0.08 bp.

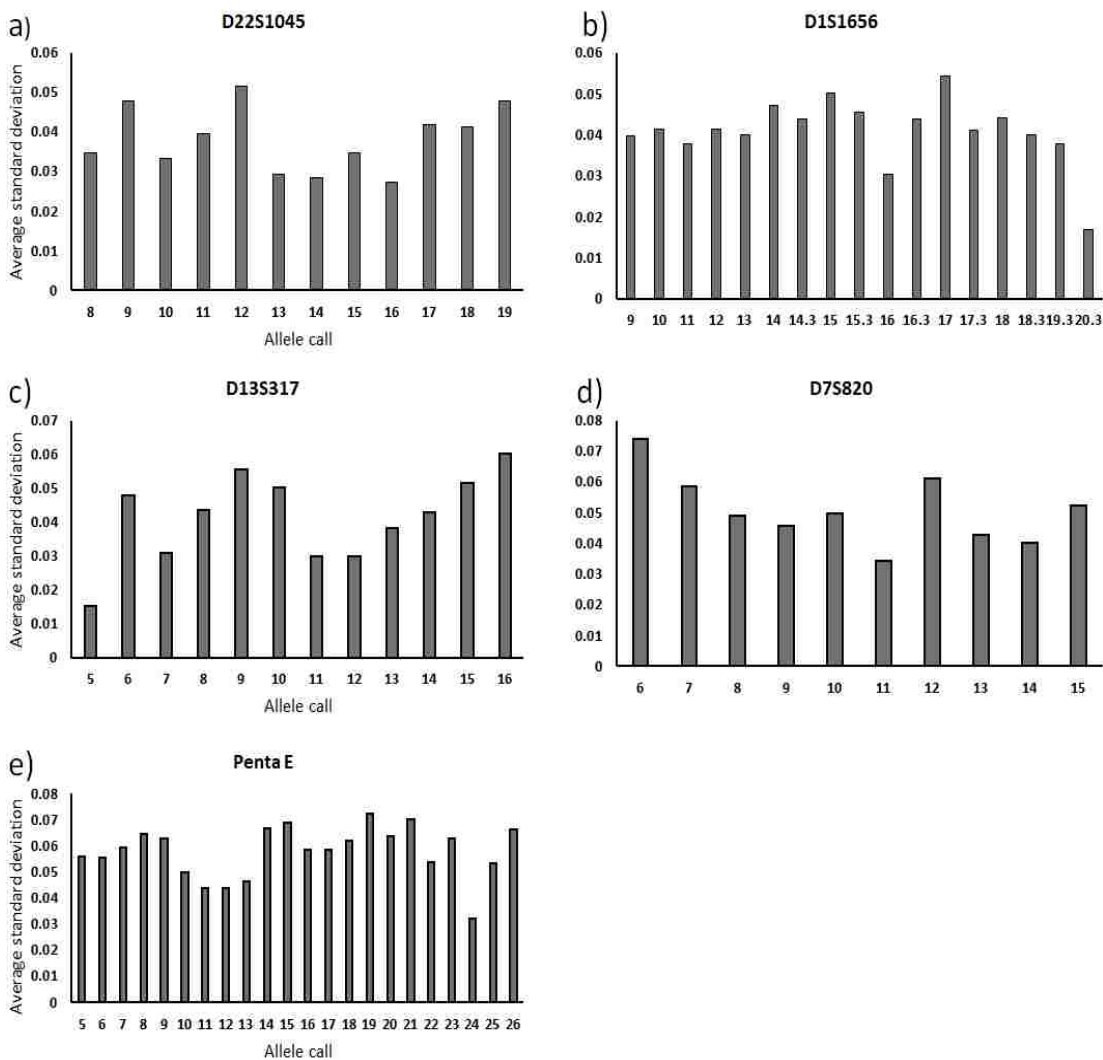


Figure 10: Allele range and detection size precision for each marker in the red dye

Figure 10 illustrates the average SD of each fragment size varies between 0.02 bp to 0.08 bp among the 5 markers in the blue dye channel.

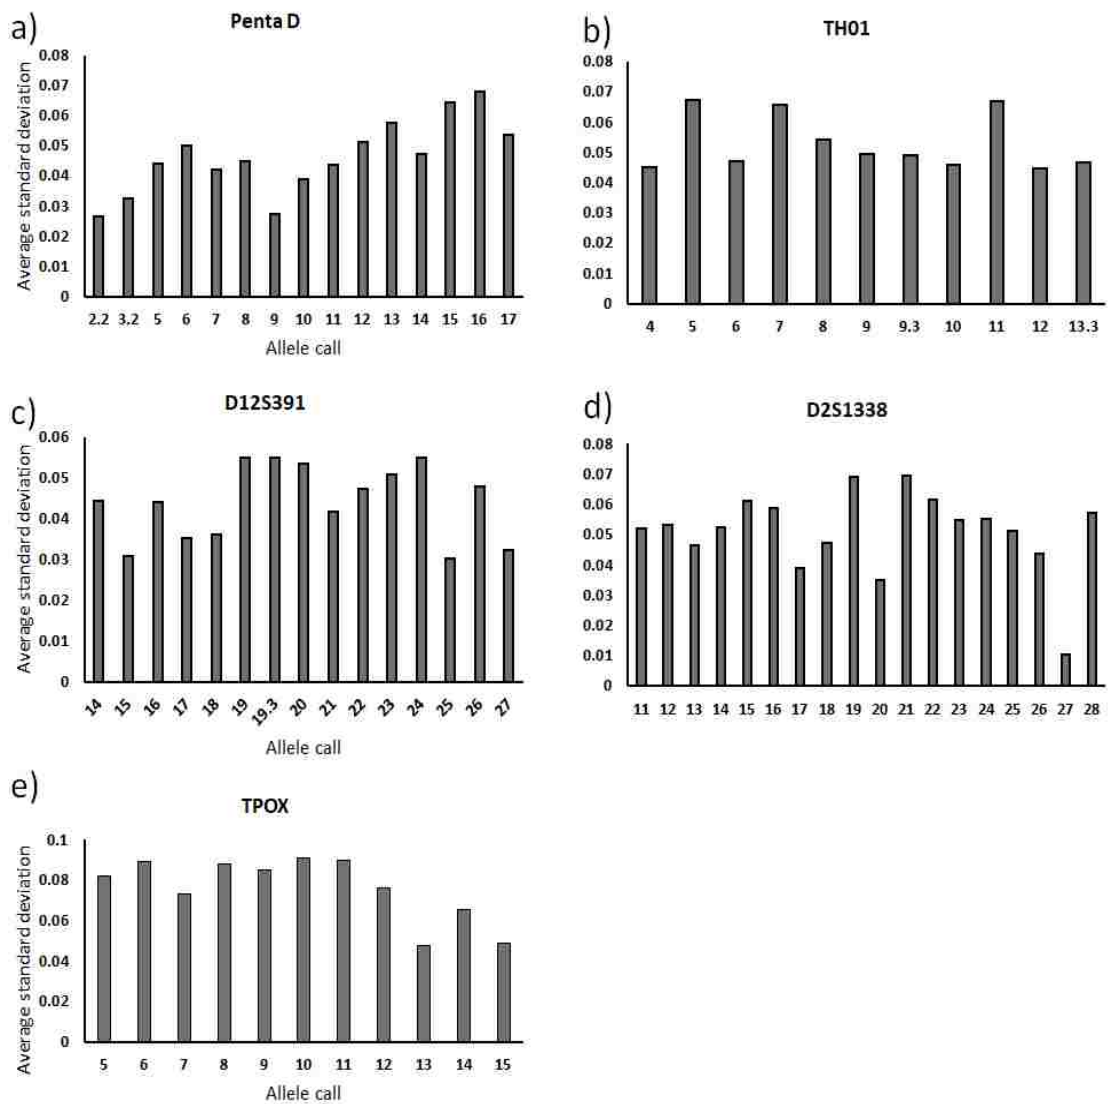


Figure 11: Allele range and detection size precision for each marker in the purple dye

Figure 11c illustrates the maximum SD which was observed for TPOX allele 10 in the purple dye channel. While the average SD of each fragment size in this dye channel varies between 0.02 bp and 0.09 bp (Figure 11).

ANOVA test was performed to compare the average size of each fragments in allelic ladder used in the precision study. Results are summarized in Table 9. F- value is less than F-critical, confirming that there is no significant difference between the mean value of fragment size in the selected allelic ladders. P-value =1 which is greater

than the confidence interval $\alpha = 0.05$, which also shows that there is no significant difference between the mean value.

Table 9: ANOVA test comparing 11 allelic ladders (AL) from one instrument

SUMMARY						
Groups	Count	Sum	Average	Variance		
AL1	362	89148.79	246.2674	9122.487		
AL2	362	89166.62	246.3166	9125.084		
AL3	362	89168.78	246.3226	9120.824		
AL4	362	89161.4	246.3022	9120.676		
AL5	362	89152.5	246.2776	9119.444		
AL6	362	89152.62	246.278	9117.448		
AL7	362	89156.5	246.2887	9120.728		
AL8	362	89157.27	246.2908	9121.239		
AL9	362	89155.43	246.2857	9118.195		
AL10	362	89157.66	246.2919	9119.563		
AL11	362	89165.3	246.313	9124.789		

ANOVA						
Source of Variation	SS	df	MS	F	P-value	F crit
Between Groups	1.12356	10	0.112356	1.23E-05	1	1.833081
Within Groups	36219302	3971	9120.952			
Total	36219303	3981				

Average SD of the fragment size was calculated for the 34 allelic ladders from multiple injection in two different instruments and the results (Table 10) support the finding in Table 9. F- value (0.000231) is less than F-critical (1.43732) and P value = 1, proving the consistency and the accuracy fragment migration among different injections.

Table 10: ANOVA test comparing 34 allelic ladders (AL) from 2 instruments

SUMMARY						
Groups	Count	Sum	Average	Variance		
AL 1	362	89148.79	246.2674	9122.487		
AL 2	362	89166.62	246.3166	9125.084		
AL 3	362	89168.78	246.3226	9120.824		
AL 4	362	89161.4	246.3022	9120.676		
AL 5	362	89152.5	246.2776	9119.444		
AL 6	362	89152.62	246.278	9117.448		
AL 7	362	89156.5	246.2887	9120.728		
AL 8	362	89157.27	246.2908	9121.239		
AL 9	362	89155.43	246.2857	9118.195		
AL 10	362	89157.66	246.2919	9119.563		
AL 11	362	89165.3	246.313	9124.789		
AL 12	362	89130.22	246.2161	9124.238		
AL 13	362	89135.45	246.2305	9122.788		
AL 14	362	89084.85	246.0907	9127.425		
AL 15	362	89135.44	246.2305	9126.821		
AL 16	362	89140.93	246.2457	9126.125		
AL 17	362	89084.97	246.0911	9130.639		
AL 18	362	89165.8	246.3144	9124.826		
AL 19	362	89134.89	246.229	9119.312		
AL 20	362	89149.51	246.2694	9121.287		
AL 21	362	89154.69	246.2837	9124.201		
AL 22	362	89136.38	246.2331	9120.749		
AL 23	362	89146.91	246.2622	9125.475		
AL 24	362	89138.05	246.2377	9120.773		
AL 25	362	89154.29	246.2826	9117.779		
AL 26	362	89180.4	246.3547	9115.658		
AL 27	362	89102.77	246.1402	9130.976		
AL 28	362	89140.33	246.244	9118.91		
AL 29	362	89174.27	246.3378	9118.941		
AL 30	362	89185.58	246.369	9117.593		
AL 31	362	89101.27	246.1361	9128.724		
AL 32	362	89190.23	246.3819	9120.295		
AL 33	362	89103.56	246.1424	9131.32		
AL 34	362	89090.07	246.1052	9130.612		
ANOVA						
Source of Variation	SS	df	MS	F	P-value	F crit
Between Groups	69.41863	33	2.103595	0.000231	1	1.43732
Within Groups	1.12E+08	12274	9122.822			
Total	1.12E+08	12307				

3.5 DNA Mixture Study

Mixture study is conducted to define and mimic the range of detectable mixture ratios, including detection of major and minor components. To assess the ability to resolve minor contributor alleles with the assay, a study was performed with nine mixture sample of male: male at different ratios (1:1, 3:1, 7:1, 10:1, 15:1 and vice versa) (Appendix 1) using standard SRM 2391c (component B and C). The total amount of mixed DNA used in this study was 500 pg (Table 11); a 15:1 mixture thus contains 30 pg of the minor component DNA and 470 pg of the major component. Samples were run in replicates of 4. The limit of detection of the minor component was determined by analyzing non-overlapping alleles of both DNAs.

Table 11 illustrates the % of detected alleles in each mixture. Full STR profile was obtained until the 1:3 ratio (130 pg for the minor contributor). 98% of expected alleles were identified for minor components of 1:7, 7:1 and 10:1 mixture, and 96% for 1:10 mixture. For 15:1 91% of the minor component alleles were identified.

Table 11: Mixture study

Mixture ratio	Total DNA input (pg)	Number of detected alleles in the mixture	% of detected alleles in the mixture
1:15	30 / 470	55/59	93
1:10	43 / 457	57/59	96.6
1:7	63 / 437	58/59	98
1:3	130 / 370	59/59	100
1:1	250 / 250	59/59	100
3:1	370 / 130	59/59	100
7:1	437/ 63	58/59	98
10:1	457 / 43	58/59	98
15:1	470 / 30	54/59	91.5

3.6 Stability Study

Two set of different PCR inhibitors was used to assess the tolerance of Verifiler™ Plus and 500 pg of control DNA 007 was used as a template. PCR was performed under standard conditions. Performance levels were assessed based on the number of alleles correctly called.

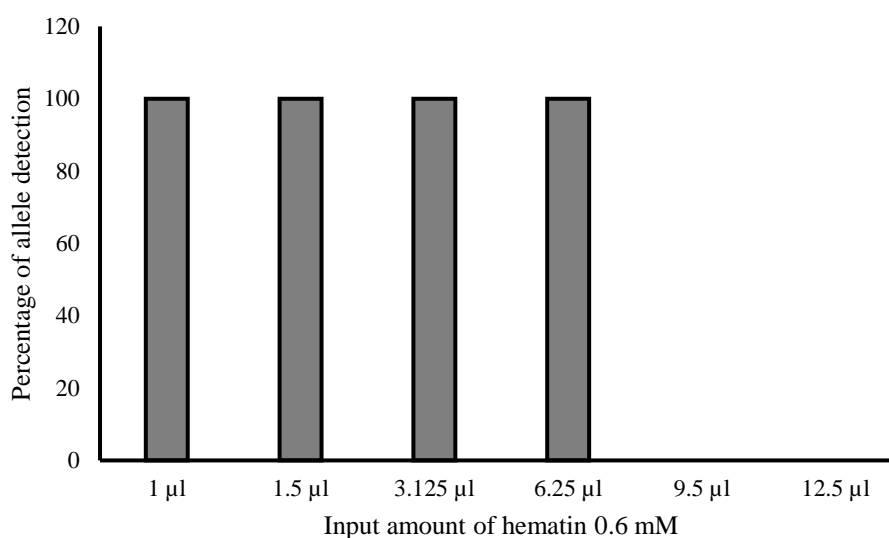


Figure 12: The effect of hematin porcine 0.6 mM on allele detection of DNA control 007

In the first set, hematin porcine (0.6mM) was added to the PCR reactions in the following amounts: 1, 1.5, 3.125, 6.25, 9.5 and 12.5 μ l. Full profile were generated in the presence of 6.25 μ l, with no alleles being detected in the presence of 9.5 μ l and 12.5 μ l (Figure 12).

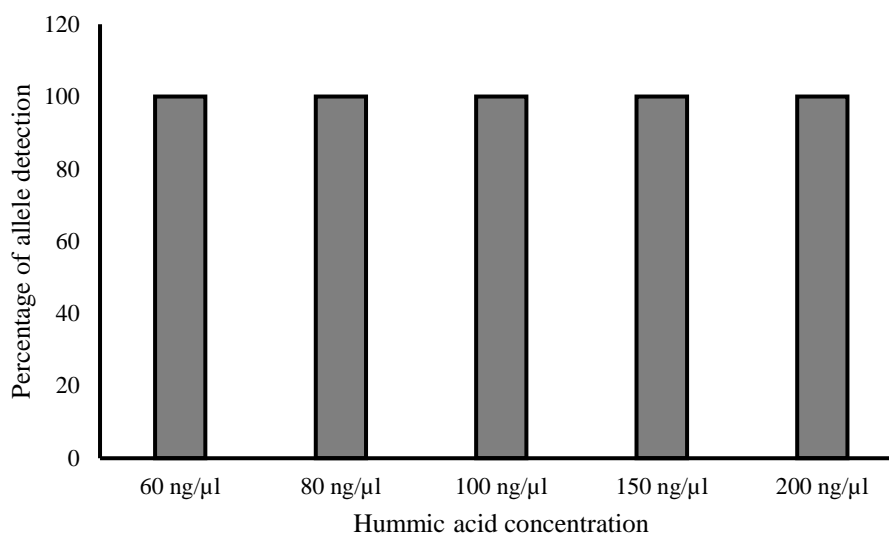


Figure 13: The effect of humic acid on allele detection of DNA control 007

In another set of experiment, humic acid was added in different concentrations ranging from 60 - 200 ng/μl. Full profiles were generated for all concentrations tested (up to 200 ng/μl) (Figure 13).

3.7 Success Rate and Concordance

Concordance study was conducted to assess the success rate of the assay. A total of 16 blood samples on FTA card, which were directly amplified, and another 16 buccal swabs along with 3 samples from the Standard Reference Materials 2391c (component A, B and C) were analyzed using this multiplex. The success rate was 100%. All genotyping was performed with GeneMapper *ID-X* v1.4 software. Data tables were exported into Microsoft Excel and compared to data generated previously with the Applied Biosystem GlobalFiler™ PCR kit. Allele call of Components A, B and C were analyzed against the certified STR allele values. All 35 samples were 100% concordance (Appendix 2).

3.8 Casework Samples

A study was performed to assess the ability to obtain reliable results from casework samples that represent the typical variation in DNA quantity and quality encountered with samples received by forensic laboratories. Different casework samples with different ranges of concentration which can impact the result and the interpretation of obtained data were selectively chose and tested to assess the performance of the assay. Eight Bn, 7 Bt, 5 CB, 1 P, 1 BI along with Ts were analyzed and compared with data previously obtained using GlobalFiler™ PCR kit (Table 12). Almost all of the samples tested yielded more alleles compared to the results previously obtained with GlobalFiler™ PCR kit (Figure 16). While the DNA concentration in swab of bottle-4 (Bt 4) (4 ng/μl) is lower than DNA concentration in cigarette butt-1 (CB 1) (8 pg/ μl), The number of allele call in (Bt 4) is significantly higher than the number obtained in (CB 1). This could be due to the presence of potential PCR inhibitors in the cigarette butt such as: tars and phenolics from the smoke, paper additives and flavor additives [26].

Table 12: Different casework samples used to assess the multiplex assay

Sample	Sample DNA pg/ μ l	Allele called		% of total alleles	
		GF	VFP	GF	VFP
CB 1	8	8	18	17	36
CB 2	400	46	49	100	100
CB 3	1200	46	49	100	100
CB 4	200	46	49	100	100
CB 5	1000	46	49	100	100
Bt 1	30	43	49	93	100
Bt 2	100	46	49	100	100
Bt 3	30	46	49	100	100
Bt 4	4	30	49	65	100
Bt 5	90	46	49	100	100
Bt 6	80	46	49	100	100
Bt 7	400	46	49	100	100
Ts	400	39	49	84	100
P	600	35	48	76	98
Bl	1400	46	49	100	100
Bn 1	60	46	49	100	100
Bn 2	20	46	49	100	100
Bn 3	30	46	49	100	100
Bn 4	30	46	49	100	100
Bn 5	30	44	49	100	100
Bn 6	16	43	46	93	94
Bn 7	20	46	49	100	100
Bn 8	500	46	49	100	100

CB: cigarette butt; Bt: bottle; Ts: human tissue; P: plug; Bl: blood; Bn: bone

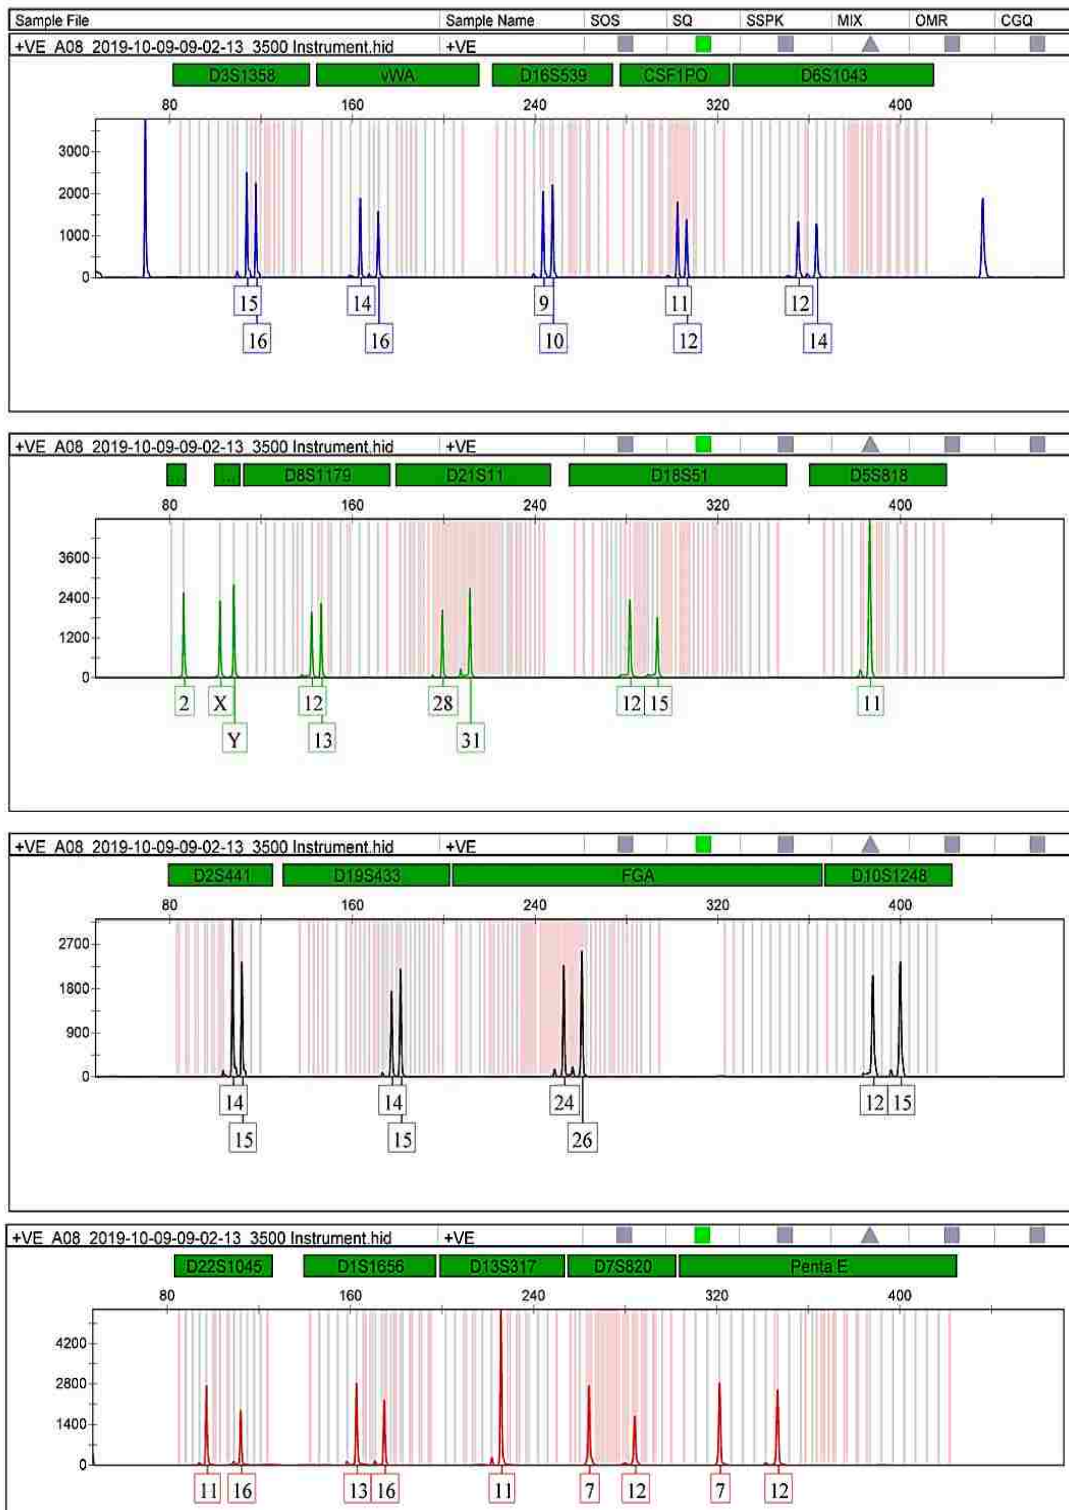


Figure 14: Electropherogram of DNA control 007 with 500 pg

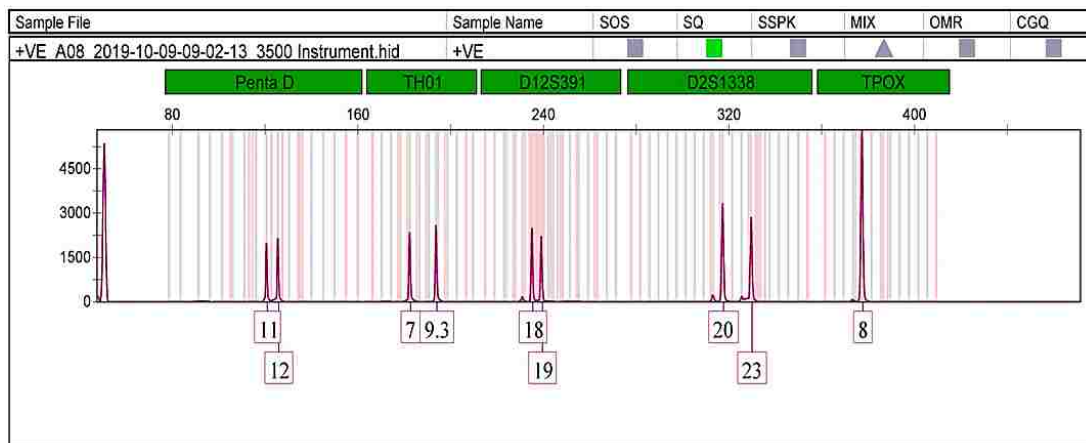


Figure 14: Electropherogram of DNA control 007 with 500 pg (Continued)

Figure 14 illustrates a full profile obtained from 500 pg of DNA control 007 which shows balanced peak height ratio.

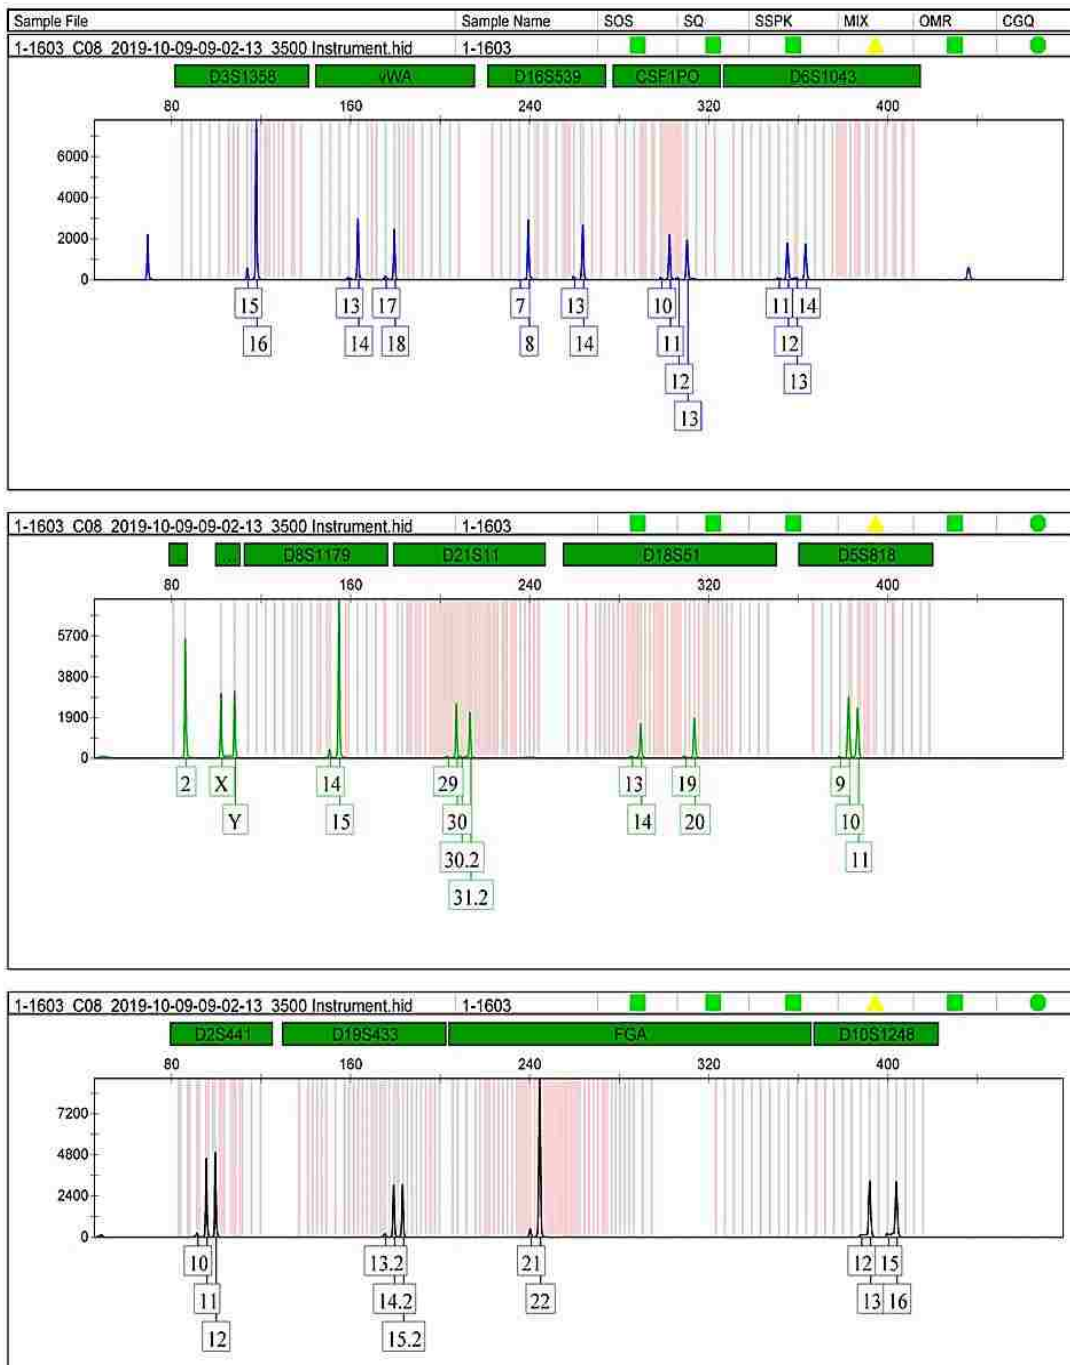


Figure 15: Electropherogram of a cigarette butt sample (1000 pg)

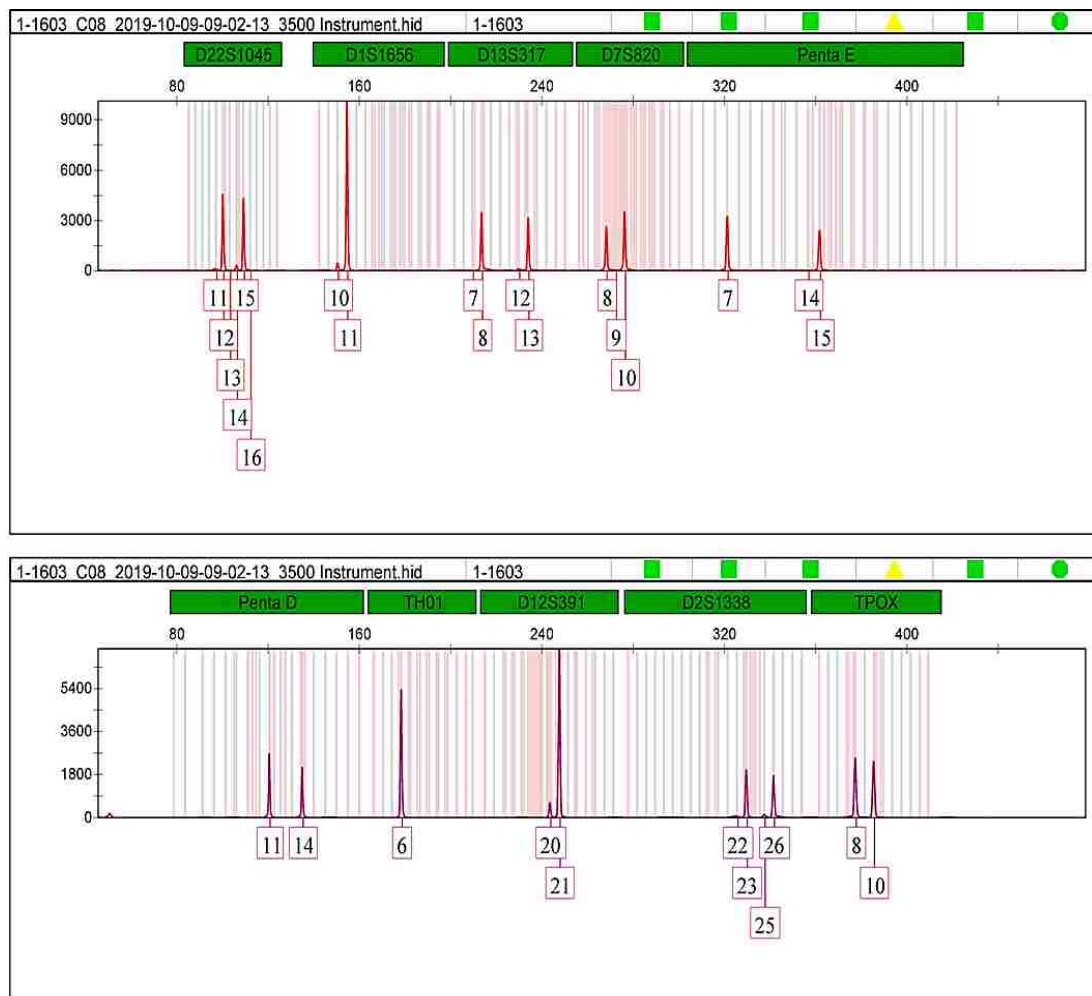


Figure 15: Electropherogram of a cigarette butt sample (1000 pg) (Continued)

Generally, profiles obtained from Verifiler™ Plus recorded higher peak heights compared to the GlobalFiler™ PCR kit (Figure 15).

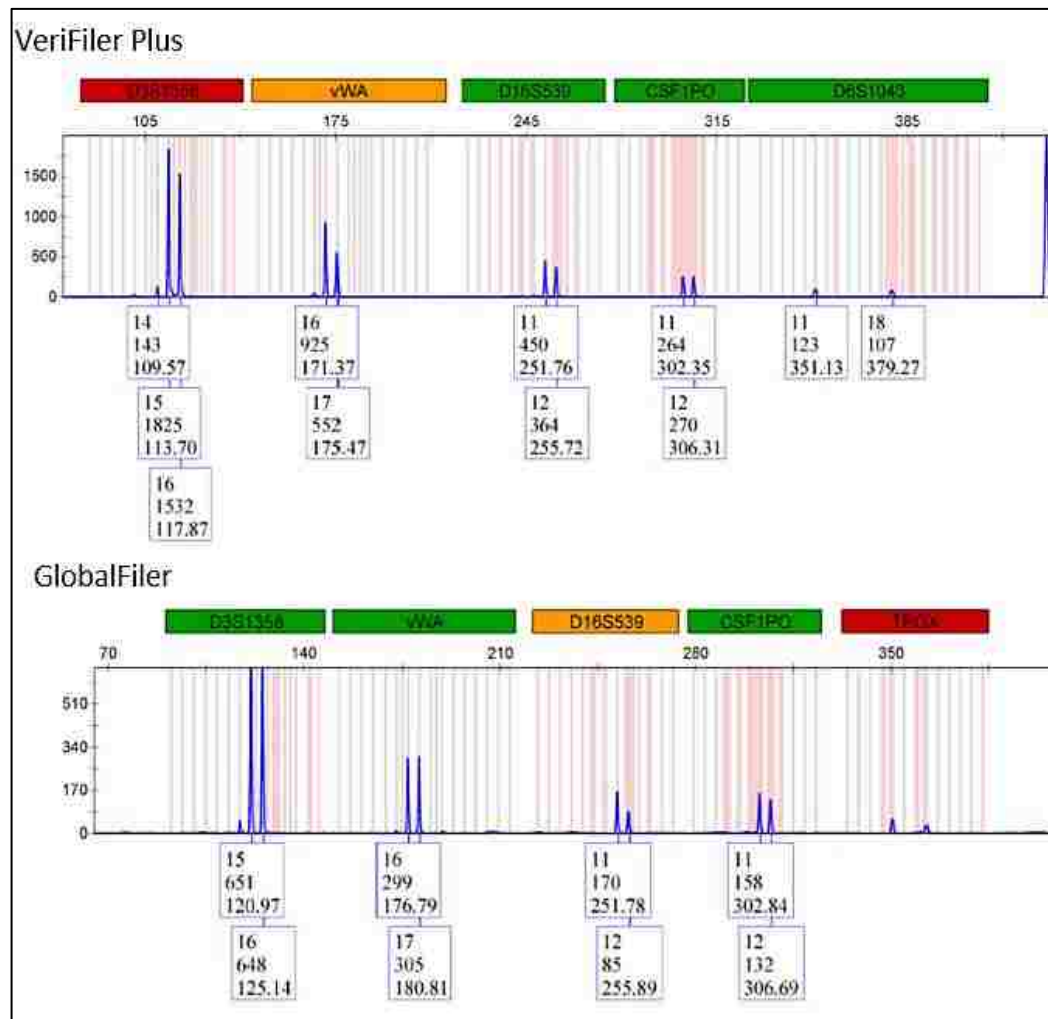


Figure 16: Electropherogram of a swab of bottle (30 pg) using two PCR assays

Figure 16 illustrates a comparison between the number of alleles generated from the same swab of bottle using VeriFiler™ Plus and GlobalFiler™ PCR kit. Results shows obtaining greater number of alleles using VeriFiler™ Plus.

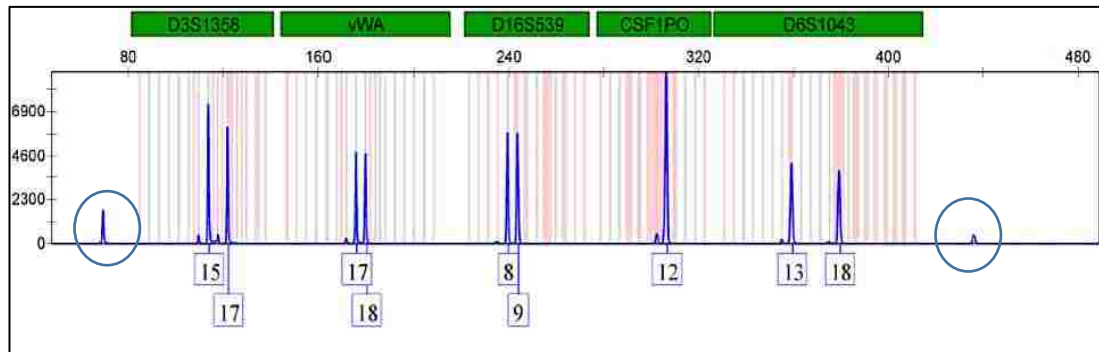


Figure 17: Illustration of two internal quality control sensors

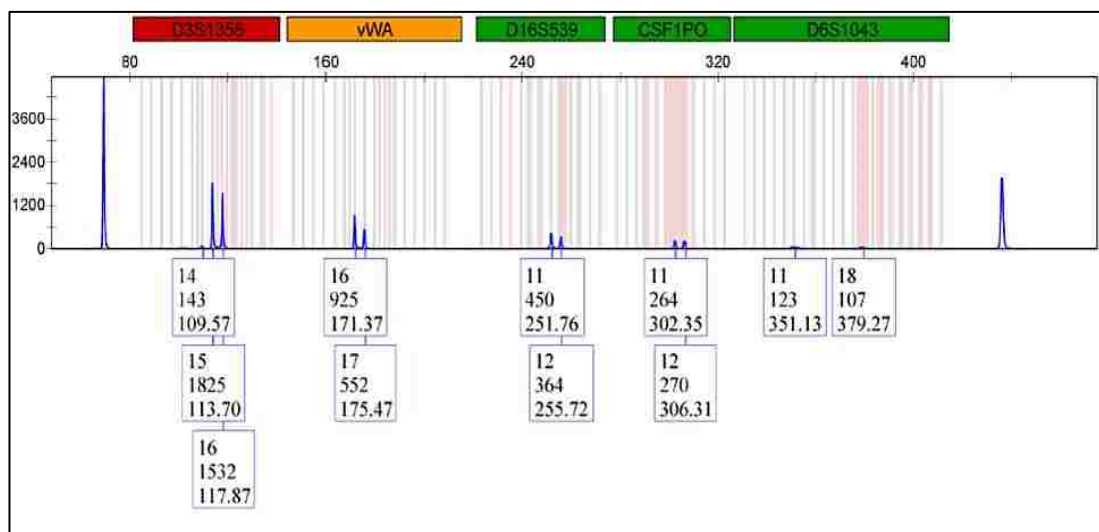


Figure 18: Interpretation of the sample in the presence of IQC

Two internal quality control sensors are included in this assay which provides extra information on the quality and the integrity of DNA sample (Figure 17). It can evaluate the PCR reaction, infer possible sample degradation or inhibition.

In Figure 18, both IQC sensors are > 2000 rfu which indicates successful PCR reaction was performed [27], while a ski slope pattern observed in the DNA profile which indicates a degradation pattern.

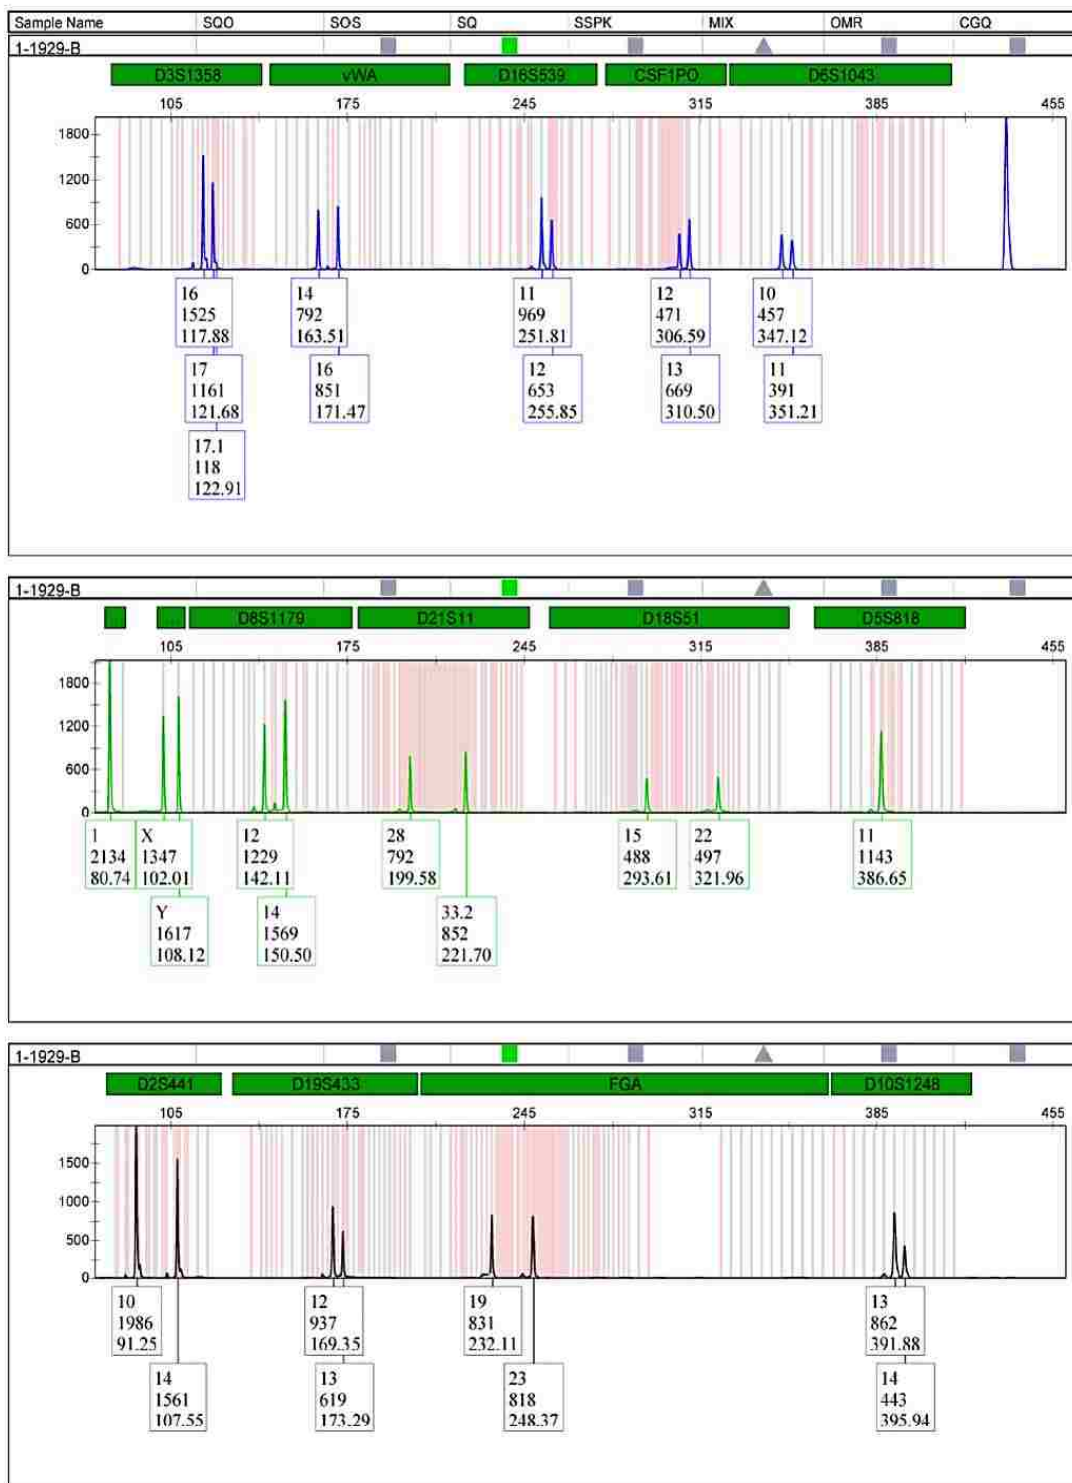


Figure 19: Electropherogram of bone sample (500 pg)

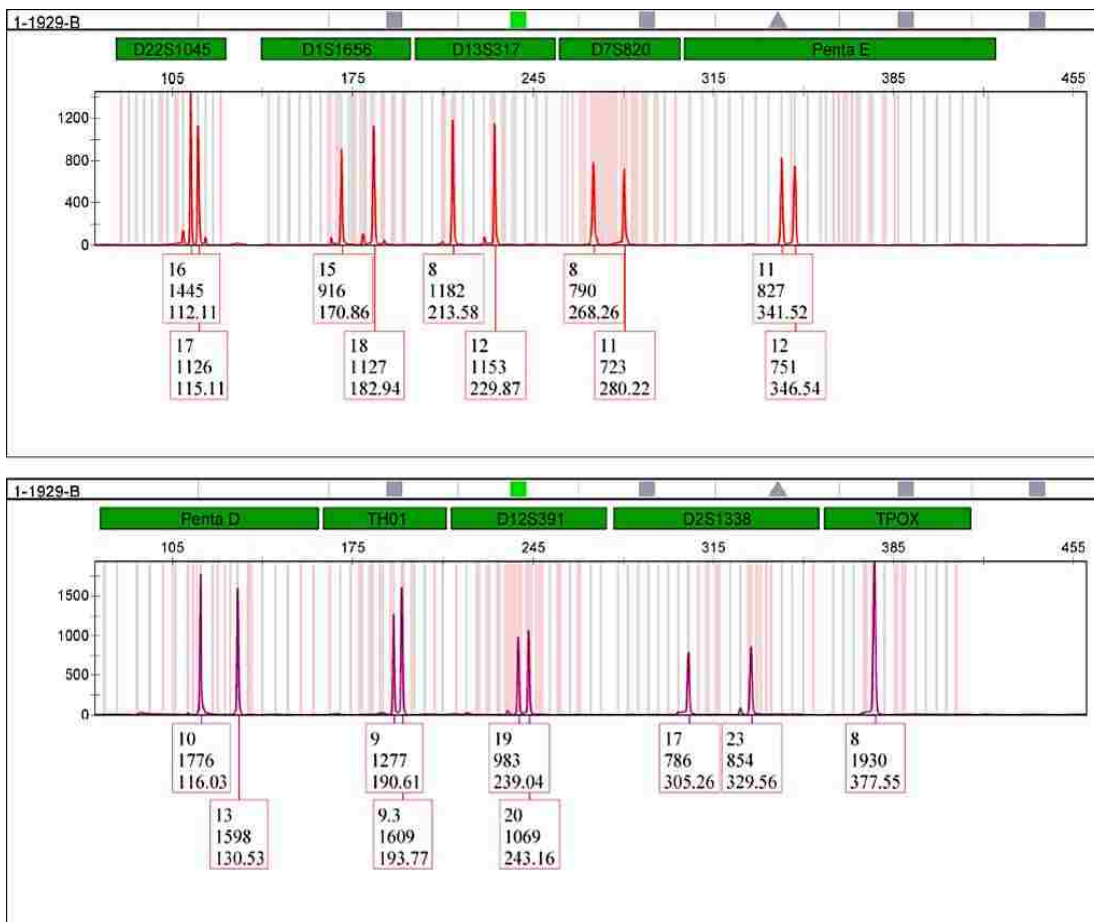


Figure 19: Electropherogram of bone sample (500 pg) (Continued)

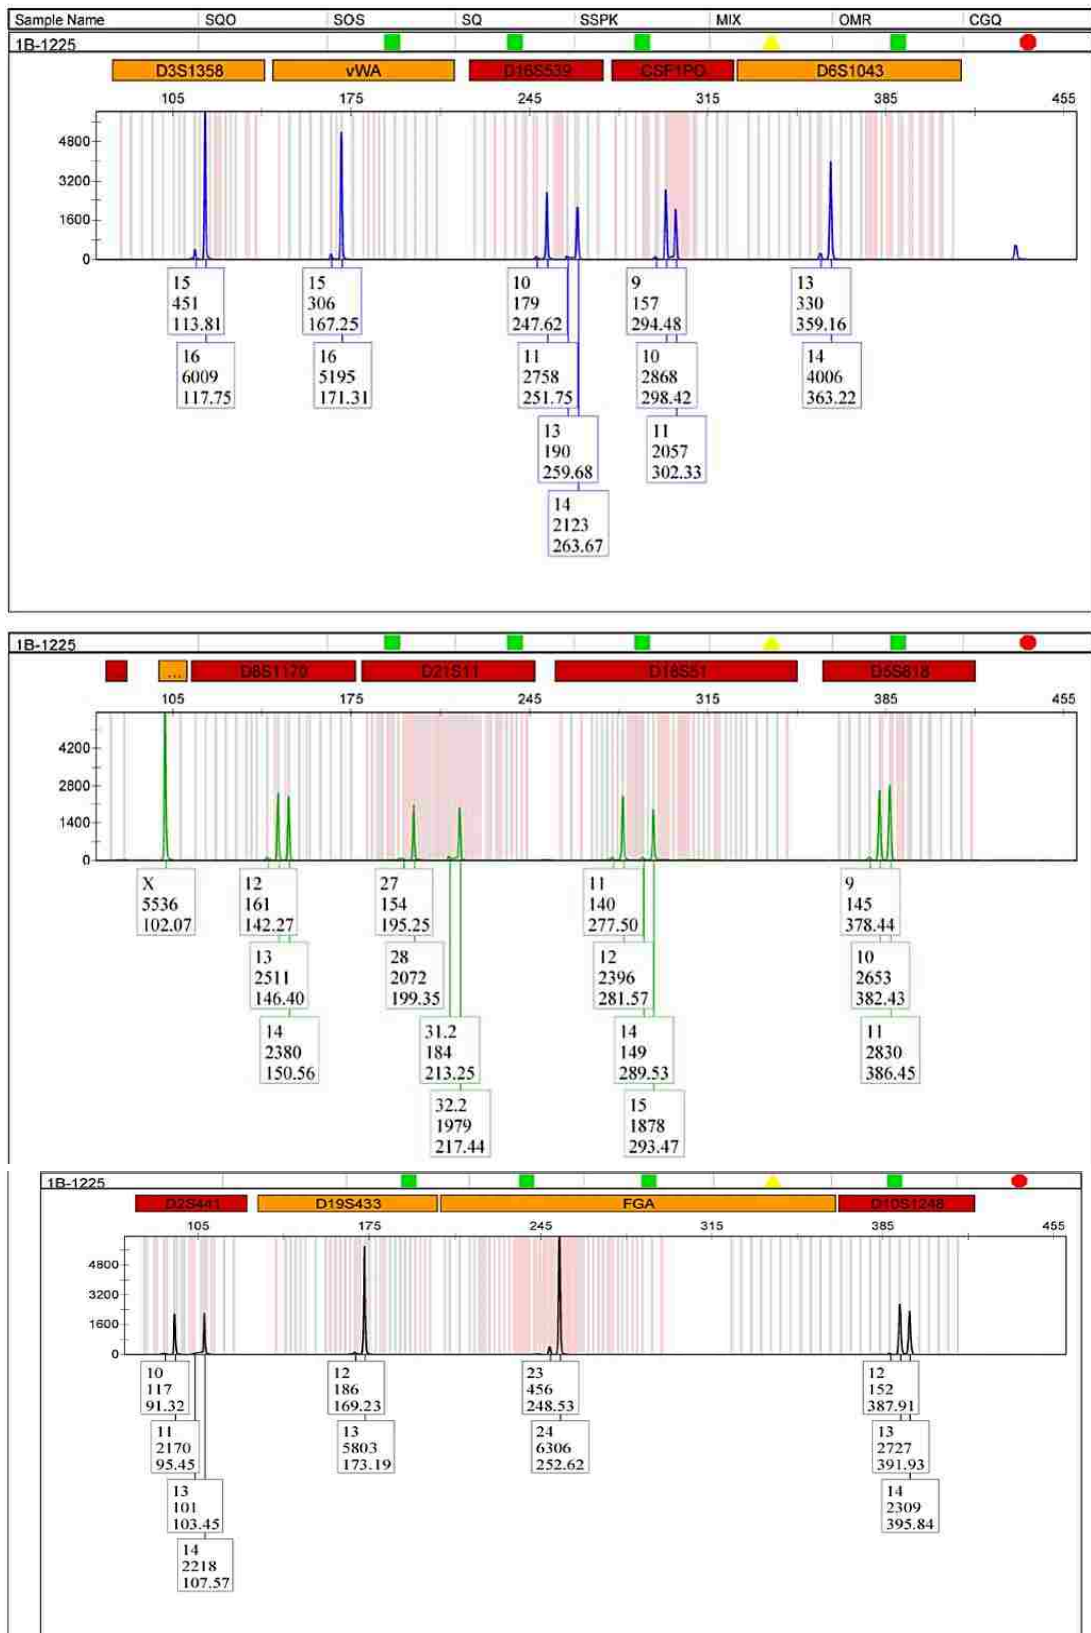


Figure 20: Electropherogram of blood sample (1400 pg)

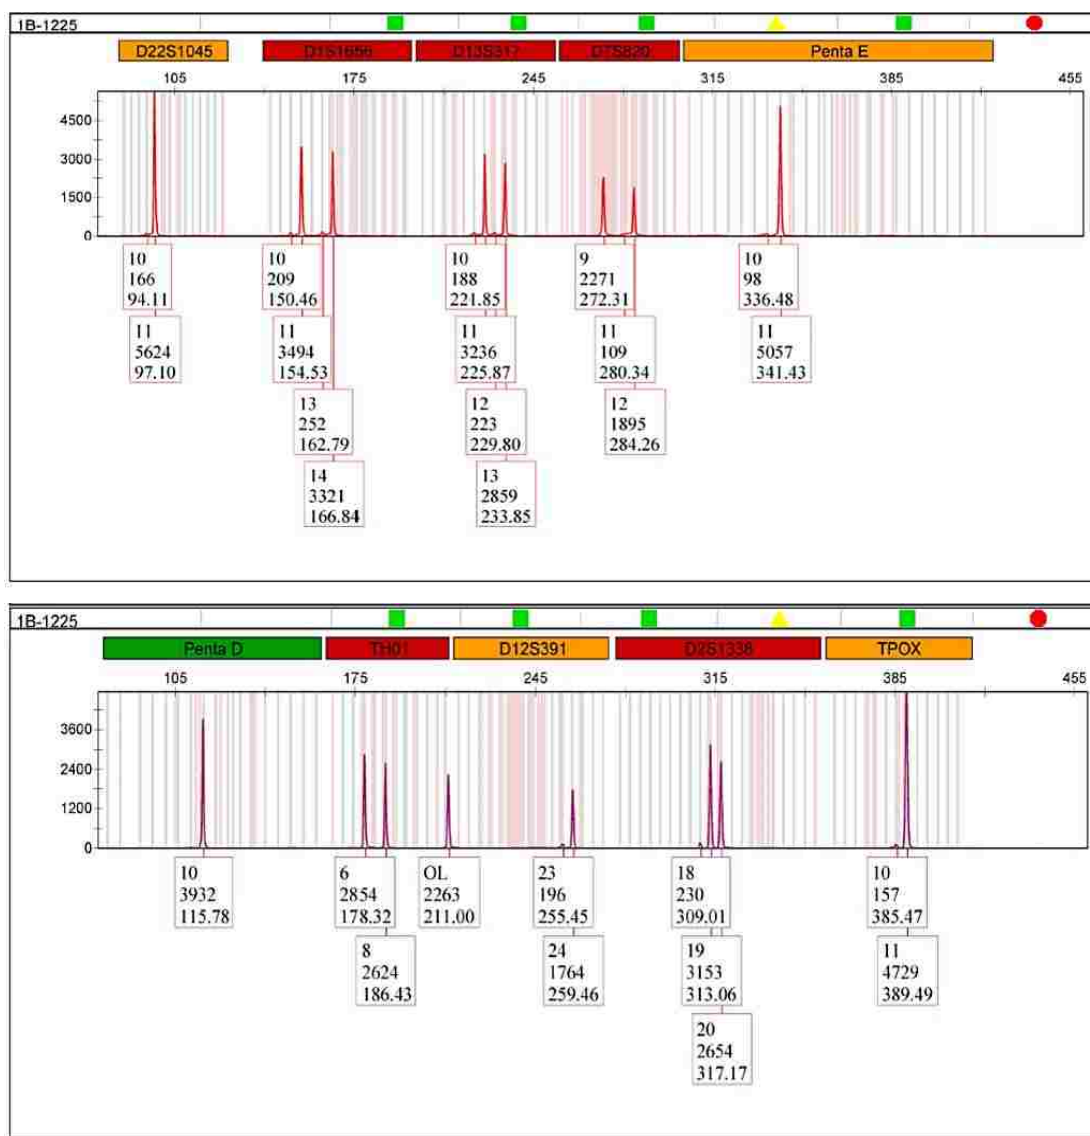


Figure 20: Electropherogram of blood sample (1400 pg) (Continued)

The main results in this study highlight the minimum DNA input required to generate a full profile is 63 pg (Figure 19). The AT was set to 80 RFU while the SD was set to 150 RFU. Size precision of Verifiler™ Plus PCR kit varied between 0.02 bp and 0.08 bp. Samples were 100% concordance and the success rate of generated profiles was 100%. The assay showed high tolerance toward humic acid (60-200 ng/ μ l) and hematin porcine (0.6 mM) (Figure 20).

Chapter 4: Discussion

This study is the first to evaluate the performance of (VeriFiler™ Plus) a six-dye STR multiplex assay with casework samples in forensic applications. Sensitivity of the assay toward DNA template input was tested and full STR profiles (100% of allele call) were obtained from all the samples ranging from 1000 pg down to 63 pg showing consistent result with a study conducted using AmpFISTR® NGM SElect™ PCR Amplification Kit [20].

However, it shows higher sensitivity compared to two other six-dye multiplexes, GlobalFiler® PCR Amplification and Investigator® 24plex QS kits [4,17, 21]. 95% of expected alleles were recovered from 32 pg DNA, which is significantly higher than the percentage of recovered allele at 32 pg in GlobalFiler® PCR Amplification [16]. 70% and 52% of all expected alleles were recovered at 16 pg and 8 pg respectively. A study reported that the Investigator® kit produced 50% of expected alleles with 8 pg of DNA [17] which is more consistent with result obtained from 8 pg DNA.

Sizing Precision is critical for determination of correct genotyping. Therefore, migration of each fragment and sizing precision must be consistent and within the bin window to ensure proper allele designation. The degree of variation generated in this study was between 0.02 bp and 0.08 bp which is within the recommended bin window for genotyping as it is mentioned by ENFSI (2010) [23] showing similar results to other studies conducted in this field [17, 25].

Mixture study can be used to assist forensic laboratories in establishing interpretation guidelines. Full STR profile was obtained until the 1:3 ratio comparing

to the results obtained from GlobalFiler Amplification kit, there is no significant difference [4].

Due to the wide range of forensic sample types and the different sampling models in the crime scene, substances known to be inhibitory toward PCR reactions are often encountered in DNA extracted from casework samples resulting either in loss of peaks or lowering of peak heights. Inhibition study was conducted to assess the tolerance and the robustness of the assay in the presence of common type of inhibitors that could bear in casework samples. Hematin porcine (0.6 mM), formed by the oxidation of heme which is the main component of blood and humic acid (60-200 ng/ μ l), a principle component of humic substances that may present in forensic samples collected from soil [17]. Full profiles were generated for all humic acid concentrations tested (up to 200 ng/ μ l). This is in agreement with findings in other studies [17]. These data demonstrate that this assay can generate a high number of alleles in the presence of the mentioned inhibitory substances.

Chapter 5: Conclusion

This study was conducted to assess and evaluate the performance of the 6-dye multiplex assay containing 23 autosomal loci with casework samples. The result of each quality control test was analyzed, sensitivity test results showed the minimum amount of DNA input resulting in a full DNA profile was 63 pg. However, the optimum range determined was 125 - 500 pg. Minimal limit of detection was calculated for every dye set, and the result obtained was used to estimate the overall analytical threshold at 80 RFU. Stochastic threshold calculation resulted in highest value to be set at 180 RFU. Heterozygous alleles were balanced for total DNA input ranging from 1000 - 500 pg while it was less than 60% for samples with total DNA input below 250 pg. All expected alleles were detected for minor contributor of 1:1, 1:3, mixture ratios, however 98% of alleles were detected for the minor contributor of 1:7, 10:1 mixture ratio. For 15:1 91% of the alleles were detected. Stability study demonstrated that this assay can generate a high number of alleles in the presence of Hematin porcine (0.6 mM) and humic acid (200 ng/ μ l). DNA profile results are concordant to those obtained from Applied Biosystem GlobalFiler™ PCR kit.

Overall, this study demonstrate that the assay can produce reliable and reproducible results, and it enhances the success rate of obtaining positive results from challenging forensic samples. This assay is fit to be used with casework samples in forensic DNA identification. Further studies are recommended to assess the resistance of this assay toward other PCR inhibitors such as inhibitors encountered in cigarette butt samples. Species specificity tests are also recommended to be done.

References

- [1] F. Gonzalez-Andrade, "Forensic Genetics Research Progress." New York, United States: Nova Science Publishers, Incorporated, 2010.
- [2] J. M. Butler, "Forensic DNA Typing: Biology, Technology, and Genetics of STR Markers." London, United States: Elsevier Science & Technology, 2005.
- [3] K. B. Gettings, R. A. Aponte, P. M. Vallone, and J. M. Butler, "STR allele sequence variation: Current knowledge and future issues," *Forensic Science International: Genetics*, vol. 18, pp. 118–130, Sep. 2015.
- [4] M. J. Ludeman, C. Zhong, J. J. Mulero, R. E. Lagace, L. K. Hennessy, M. L. Short, D. Y. Wang, "Developmental validation of GlobalFiler™ PCR amplification kit: a 6-dye multiplex assay designed for amplification of casework samples," *Int J Legal Med*, vol. 132, no. 6, pp. 1555–1573, Nov. 2018.
- [5] D. R. Hares, "Addendum to expanding the CODIS core loci in the United States," *Forensic Science International: Genetics*, vol. 6, no. 5, p. 135–145, Sep. 2012.
- [6] M. Kayser and P. de Knijff, "Improving human forensics through advances in genetics, genomics and molecular biology," *Nature Reviews Genetics*, vol. 12, no. 3, pp. 179–192, Mar. 2011.
- [7] A. McDonald, E. Jones, J. Lewis, and P. O'Rourke, "Y-STR analysis of digital and/or penile penetration cases with no detected spermatozoa," *Forensic Science International: Genetics*, vol. 15, pp. 84–89, Mar. 2015.
- [8] S. T. G. Ferreira, K. A. Paula, F. A. Maia, A. E. Svidizinski, M. R. Amaral, S. A. Diniz, M. E. Siqueira, A. V. Moraes, L. Gusmao, L. Roewer, "Routine analysis of sexual assault cases in Brasília, Brazil, using 23 Y chromosomal markers," *Forensic Science International: Genetics Supplement Series*, vol. 5, pp. 619–621, Dec. 2015.
- [9] I. Pickrahn, E. Muller, W. Zahrer, B. Dunkelmann, J. Kiesslich, G. Kreindl, F. Neuhuber, "Yfiler® Plus amplification kit validation and calculation of forensic parameters for two Austrian populations," *Forensic Science International: Genetics*, vol. 21, pp. 90–94, Mar. 2016.
- [10] Y. Ye, J. Gao, G. Fan, L. Liao, and Y. Hou, "Population genetics for 23 Y-STR loci in Tibetan in China and confirmation of DYS448 null allele," *Forensic Science International: Genetics*, vol. 16, pp. 7–10, May 2015.

- [11] S. Palomo-Díez, C. Gomes, Á. Esparza-Arroyo, and E. Arroyo-Pardo, “Comparison of three commercial kits to the establishment of str genetic profiles on critical samples,” *Forensic Science International: Genetics Supplement Series*, vol. 6, pp. 200–202, Dec. 2017.
- [12] R. Alaeddini, “Forensic implications of PCR inhibition—A review,” *Forensic Science International: Genetics*, vol. 6, no. 3, pp. 297–305, May 2012.
- [13] K. Elwick, X. Zeng, J. King, B. Budowle, and S. Hughes-Stamm, “Comparative tolerance of two massively parallel sequencing systems to common PCR inhibitors,” *International Journal of Legal Medicine; Heidelberg*, vol. 132, no. 4, pp. 983–995, Jul. 2018.
- [14] P. Rådström, R. Knutsson, P. Wolffs, M. Lövenklev, and C. Löfström, “Pre-PCR processing: Strategies to generate PCR-compatible samples,” *Molecular Biotechnology; Totowa*, vol. 26, no. 2, pp. 133–146, Feb. 2004.
- [15] T. Senge, B. Madea, A. Junge, M. A. Rothschild, and P. M. Schneider, “STRs, mini STRs and SNPs – A comparative study for typing degraded DNA,” *Legal Medicine*, vol. 13, no. 2, pp. 68–74, Mar. 2011.
- [16] P. Martín, L. F. de Simón, G. Luque, M. J. Farfán, and A. Alonso, “Improving DNA data exchange: Validation studies on a single 6 dye STR kit with 24 loci,” *Forensic Science International: Genetics*, vol. 13, pp. 68–78, Nov. 2014.
- [17] M. Kraemer, A. Prochnow, M. Bussmann, M. Scherer, R. Peist, and C. Steffen, “Developmental validation of QIAGEN Investigator[®] 24plex QS Kit and Investigator[®] 24plex GO! Kit: Two 6-dye multiplex assays for the extended CODIS core loci,” *Forensic Science International: Genetics*, vol. 29, pp. 9–20, Jul. 2017.
- [18] M. G. Ensenberger, K. A. Lenz, L. K. Mattheis, G. M. Hadinoto, J. E. Schienman, A. J. Przech, M. W. Morganti, D. T. Renstorm, V. M. Baker, K. M. Gawrys, M. Hoogendoorn, C. R. Steffen, P. Martin, A. Alonso, H. R. Olson, C. J. Sprecher, D. R. Storts, “Developmental validation of the PowerPlex[®] Fusion 6C System,” *Forensic Science International: Genetics*, vol. 21, pp. 134–144, Mar. 2016.
- [19] S. Lin, C. Li, and S. C. Y. Ip, “A selection guide for the new generation 6-dye DNA profiling systems,” *Forensic Science International: Genetics*, vol. 30, pp. 34–42, Sep. 2017.
- [20] A. Barbaro, P. Cormaci, and A. Agostino, “Validation of AmpFLSTR NGM SElect[™] PCR amplification kit on forensic samples,” *Forensic Science International: Genetics Supplement Series*, vol. 3, no. 1, pp. 67–68, Dec. 2011.

- [21] K. Elwick, C. Mayes, and S. Hughes-Stamm, “Comparative sensitivity and inhibitor tolerance of GlobalFiler® PCR Amplification and Investigator® 24plex QS kits for challenging samples,” *Legal Medicine*, vol. 32, pp. 31–36, May 2018.
- [22] SWGDAM, “Swgdam Interpretation Guidelines for Autosomal STR typing by Forensic DNA Testing Laboratories.” Accessed on: October 16, 2019, Accessed at: http://www.forensicdna.com/assets/swgdam_2010.pdf
- [23] ENFSI, “Minimum Validation Guidelines in DNA Profiling.” Accessed on: October 16, 2019, Accessed at: http://enfsi.eu/wp-content/uploads/2016/09/minimum_validation_guidelines_in_dna_profiling_-_v2010_0.pdf.
- [24] J. M. Butler, “Advanced Topics in Forensic DNA Typing: Methodology.” San Diego, United States: Elsevier Science & Technology, 2011.
- [25] R. S. McLaren, J. Heller, J. Patel, J. M. Thompson, J. Pagram, T. Loake, D. Beesley, M. Prittimaa, C. R. Hill, D. L. Duewer, M. C. Kline, J. M. Butler, D. R. Storts, “Developmental validation of the PowerPlex® ESI 16/17 Fast and PowerPlex® ESX 16/17 Fast Systems,” *Forensic Science International: Genetics*, vol. 13, pp. 195–205, Nov. 2014.
- [26] L. Casey, S. Engen, and G. Frank, “Quantitative Analysis of the DNA Distribution on Cigarette Butt Filter Paper,” *Journal of Forensic Sciences*, vol. 58, no. 2, pp. 470–473, Dec. 2013.
- [27] Thero Fisher, “VeriFiler™ Plus PCR Amplification Kit USER GUIDE.” Accessed on: October 5, 2018, Accessed at: https://assets.thermofisher.com/TFS-Assets/LSG/manuals/MAN0017493_VeriFilerPlusPCRAmpKit_UG.pdf

Appendix

(1)

- Sample setup for Mixture study using Component B and C (1.6 ng/ μ l)
 - Samples were diluted to reach a final concentration of 0.5 ng/ μ l in 100 μ l. To prepare a stock solution for each component (B & C), 31.25 μ l was added to 68.75 μ l of the diluent.
 - Mixtures were prepared using the following amounts:

Table 13: Volume of each diluted DNA sample required to prepare mixture set 1

Ratio	Volume of B (μl)	Volume of C (μl)
1:1	8.75	8.75
3:1	13.1	4.4
7:1	15.3	2.2
10:1	16	1.5
15:1	16.5	1

Table 14: Volume of each diluted DNA sample required to prepare mixture set 2

Ratio	Volume of C (μl)	Volume of B (μl)
1:3	13.1	4.4
1:7	15.3	2.2
1:10	16	1.5
1:15	16.5	1

(2)

Table 15: Concordance study with SRM 2391c samples (component A, B and C)

sample	markers	Verifiler Plus		Certificate of Ananlysis- Standard Reference Material 2391c	
A	D3S1358	15	16	15	16
	vWA	18	19	18	19
	D16S539	10	11	10	11
	CSF1PO	10	10	10	10
	D6S1043	11	18	11	18
	Yindel				
	AMEL	X	X	X	X
	D8S1179	13	14	13	14
	D21S11	28	32.2	28	32.2
	D18S51	12	15	12	15
	D5S818	11	12	11	12
	D2S441	10	10	10	10
	D19S433	13	14	13	14
	FGA	21	23	21	23
	D10S1248	15	16	15	16
	D22S1045	15	15	15	15
	D1S1656	17.3	17.3	17.3	17.3
	D13S317	8	8	8	8
	D7S820	11	11	11	11
	Penta E	5	10	5	10
	Penta D	9	13	9	13
	TH01	8	9.3	8	9.3
	D12S391	18.3	22	18.3	22
	D2S1338	18	23	18	23
TPOX	8	8	8	8	
B	D3S1358	15	19	15	19
	vWA	17	18	17	18
	D16S539	10	13	10	13
	CSF1PO	10	11	10	11
	D6S1043	14	19	14	19
	Yindel	2			
	AMEL	X	Y	X	Y
	D8S1179	10	13	10	13
	D21S11	32	32.2	32	32.2
	D18S51	13	16	13	16
	D5S818	12	13	12	13
	D2S441	10	14	10	14
	D19S433	16	16.2	16	16.2
	FGA	20	23	20	23

Table 15: Concordance study with SRM 2391c sample (component A, B and C)
(continued)

sample	markers	Verifiler Plus		Certificate of Ananalysis- Standard Reference Material 2391c		
B	D10S1248	13	13	13	13	
	D22S1045	15	17	15	17	
	D1S1656	11	14	11	14	
	D13S317	9	12	9	12	
	D7S820	10	10	10	10	
	Penta E	7	15	7	15	
	Penta D	8	12	8	12	
	TH01	6	9.3	6	9.3	
	D12S391	19	24	19	24	
	D2S1338	17	17	17	17	
	TPOX	8	11	8	11	
	C	D3S1358	16	18	16	18
		vWA	16	18	16	18
D16S539		10	10	10	10	
CSF1PO		10	12	10	12	
D6S1043		11	14	11	14	
Yindel		2				
AMEL		X	Y	X	Y	
D8S1179		10	17	10	17	
D21S11		29	30	29	30	
D18S51		16	19	16	19	
D5S818		10	11	10	11	
D2S441		10	10	10	10	
D19S433		13.2	15.2	13.2	15.2	
FGA		24	26	24	26	
D10S1248		12	16	12	16	
D22S1045		16	16	16	16	
D1S1656		11	15	11	15	
D13S317		11	11	11	11	
D7S820		10	12	10	12	
Penta E		12	13	12	13	
Penta D		10	11	10	11	
TH01		6	8	6	8	
D12S391		19	23	19	23	
D2S1338		19	19	19	19	
TPOX		11	11	11	11	

Table 16: Concordance study with blood and buccal swab samples using GlobalFiler (GF) and Verifiler Plus (VFP) PCR kits

Sample	markers	GF		markers	VFP- Blood		VFP- Buccal swab		
1	D3S1358	15	18	D3S1358	15	18	15	18	
	vWA	15	17	vWA	15	17	15	17	
	D16S539	10	12	D16S539	10	12	10	12	
	CSF1PO	11	12	CSF1PO	11	12	11	12	
	TPOX	8	8	D6S1043	12	17	12	17	
	Yindel	2		Yindel	2		2		
	AMEL	X	Y	AMEL	X	Y	X	Y	
	D8S1179	14	14	D8S1179	14	14	14	14	
	D21S11	28	29	D21S11	28	29	28	29	
	D18S51	14	14	D18S51	14	14	14	14	
	DYS391	10	10	D5S818	11	12	11	12	
	D2S441	10	14	D2S441	10	14	10	14	
	D19S433	14	15	D19S433	14	15	14	15	
	TH01	7	8	FGA	21	24	21	24	
	FGA	21	24	D10S1248	15	16	15	16	
	D22S1045	11	15	D22S1045	11	15	11	15	
	D5S818	11	12	D1S1656	17	17.3	17	17.3	
	D13S317	11	13	D13S317	11	13	11	13	
	D7S820	10	11	D7S820	10	11	10	11	
	SE33	19	27.2	Penta E	7	10	7	10	
	D10S1248	15	16	Penta D	11	12	11	12	
	D1S1656	17	17.3	TH01	7	8	7	8	
	D12S391	22	24	D12S391	22	24	22	24	
	D2S1338	18	23	D2S1338	18	23	18	23	
				TPOX	8	8	8	8	
	2	D3S1358	15	15	D3S1358	15	15	15	15
		vWA	17	18	vWA	17	18	17	18
		D16S539	9	13	D16S539	9	13	9	13
		CSF1PO	12	12	CSF1PO	12	12	12	12
		TPOX	8	11	D6S1043	11	14	11	14
Yindel				Yindel					
AMEL		X	X	AMEL	X	X	X	X	
D8S1179		12	13	D8S1179	12	13	12	13	
D21S11		28	30	D21S11	28	30	28	30	
D18S51		12	14	D18S51	12	14	12	14	
DYS391				D5S818	12	13	12	13	
D2S441		11	11	D2S441	11	11	11	11	
D19S433		13	14	D19S433	13	14	13	14	
TH01		6	7	FGA	19	25	19	25	
FGA		19	25	D10S1248	13	14	13	14	
D22S1045	11	15	D22S1045	11	15	11	15		

Table 16: Concordance study with blood and buccal swab samples using GlobalFiler (GF) and Verifiler Plus (VFP) PCR kits (continued)

Sample	markers	GF		markers	VFP- Blood		VFP- Buccal swab	
	D5S818	12	13	D1S1656	12	16	12	16
	D13S317	12	12	D13S317	12	12	12	12
	D7S820	8	11	D7S820	8	11	8	11
	SE33	28.2	29.2	Penta E	5	19	5	19
	D10S1248	13	14	Penta D	12	14	12	14
	D1S1656	12	16	TH01	6	7	6	7
	D12S391	18	18	D12S391	18	18	18	18
	D2S1338	17	19	D2S1338	17	19	17	19
				TPOX	8	11	8	11
3	D3S1358	15	18	D3S1358	15	18	15	18
	vWA	17	18	vWA	17	18	17	18
	D16S539	12	13	D16S539	12	13	12	13
	CSF1PO	11	12	CSF1PO	11	12	11	12
	TPOX	8	8	D6S1043	11	13	11	13
	Yindel			Yindel				
	AMEL	X	X	AMEL	X	X	X	X
	D8S1179	15	16	D8S1179	15	16	15	16
	D21S11	29	31	D21S11	29	31	29	31
	D18S51	16	17	D18S51	16	17	16	17
	DYS391			D5S818	12	13	12	13
	D2S441	11	14	D2S441	11	14	11	14
	D19S433	15	15.2	D19S433	15	15.2	15	15.2
	TH01	6	6	FGA	22	22	22	22
	FGA	22	22	D10S1248	14	15	14	15
	D22S1045	15	16	D22S1045	15	16	15	16
	D5S818	12	13	D1S1656	11	17	11	17
	D13S317	8	13	D13S317	8	13	8	13
	D7S820	10	11	D7S820	10	11	10	11
	SE33	23.2	36	Penta E	12	13	12	13
	D10S1248	14	15	Penta D	11	14	11	14
	D1S1656	11	17	TH01	6	6	6	6
	D12S391	17	18	D12S391	17	18	17	18
	D2S1338	19	19	D2S1338	19	19	19	19
				TPOX	8	8	8	8
4	D3S1358	15	18	D3S1358	15	18	15	18
	vWA	17	18	vWA	17	18	17	18
	D16S539	12	12	D16S539	12	12	12	12
	CSF1PO	12	12	CSF1PO	12	12	12	12
	TPOX	8	11	D6S1043	11	19	11	19
	Yindel			Yindel				
	AMEL	X	X	AMEL	X	X	X	X

Table 16: Concordance study with blood and buccal swab samples using GlobalFiler (GF) and Verifiler Plus (VFP) PCR kits (continued)

Sample	markers	GF		markers	VFP- Blood		VFP- Buccal swab	
	D8S1179	12	13	D8S1179	12	13	12	13
	D21S11	29	29	D21S11	29	29	29	29
	D18S51	14	15	D18S51	14	15	14	15
	DYS391			D5S818	13	13	13	13
	D2S441	11	14	D2S441	11	14	11	14
	D19S433	13	14	D19S433	13	14	13	14
	TH01	6	9	FGA	21	23	21	23
	FGA	21	23	D10S1248	14	15	14	15
	D22S1045	15	15	D22S1045	15	15	15	15
	D5S818	13	13	D1S1656	15	17.3	15	17.3
	D13S317	11	12	D13S317	11	12	11	12
	D7S820	9	11	D7S820	9	11	9	11
	SE33	18	21.1	Penta E	5	13	5	13
	D10S1248	14	15	Penta D	9	9	9	9
	D1S1656	15	17.3	TH01	6	9	6	9
	D12S391	20	23	D12S391	20	23	20	23
	D2S1338	17	21	D2S1338	17	21	17	21
				TPOX	8	11	8	11
5	D3S1358	16	17	D3S1358	16	17	16	17
	vWA	17	17	vWA	17	17	17	17
	D16S539	10	14	D16S539	10	14	10	14
	CSF1PO	11	12	CSF1PO	11	12	11	12
	TPOX	8	8	D6S1043	11	11	11	11
	Yindel			Yindel				
	AMEL	X	X	AMEL	X	X	X	X
	D8S1179	11	13	D8S1179	11	13	11	13
	D21S11	29	32.2	D21S11	29	32.2	29	32.2
	D18S51	16	18	D18S51	16	18	16	18
	DYS391			D5S818	10	11	10	11
	D2S441	10	12	D2S441	10	12	10	12
	D19S433	13	14	D19S433	13	14	13	14
	TH01	6	9	FGA	20	23	20	23
	FGA	20	23	D10S1248	15	15	15	15
	D22S1045	11	15	D22S1045	11	15	11	15
	D5S818	10	11	D1S1656	11	17.3	11	17.3
	D13S317	14	14	D13S317	14	14	14	14
	D7S820	9	10	D7S820	9	10	9	10
	SE33	18	20.2	Penta E	7	OL	7	OL
	D10S1248	15	15	Penta D	11	12	11	12
	D1S1656	11	17.3	TH01	6	9	6	9
	D12S391	18.3	21	D12S391	18.3	21	18.3	21

Table 16: Concordance study with blood and buccal swab samples using GlobalFiler (GF) and Verifiler Plus (VFP) PCR kits (continued)

Sample	markers	GF		markers	VFP- Blood		VFP- Buccal swab	
6	D2S1338	19	19	D2S1338	19	19	19	19
				TPOX	8	8	8	8
	D3S1358	17	18	D3S1358	17	18	17	18
	vWA	14	14	vWA	14	14	14	14
	D16S539	9	9	D16S539	9	9	9	9
	CSF1PO	10	12	CSF1PO	10	12	10	12
	TPOX	8	8	D6S1043	12	18	12	18
	Yindel			Yindel				
	AMEL	X	X	AMEL	X	X	X	X
	D8S1179	13	13	D8S1179	13	13	13	13
	D21S11	31	32	D21S11	31	32	31	32
	D18S51	12	16	D18S51	12	16	12	16
	DYS391			D5S818	10	12	10	12
	D2S441	10	12	D2S441	10	12	10	12
	D19S433	13.2	14	D19S433	13.2	14	13.2	14
	TH01	9	9	FGA	21	24	21	24
	FGA	21	24	D10S1248	13	14	13	14
	D22S1045	15	15	D22S1045	15	15	15	15
	D5S818	10	12	D1S1656	16	16	16	16
	D13S317	9	12	D13S317	9	12	9	12
	D7S820	11	13	D7S820	11	13	11	13
	SE33	25.2	27.2	Penta E	11	17	11	17
	D10S1248	13	14	Penta D	10	11	10	11
	D1S1656	16	16	TH01	9	9	9	9
	D12S391	18	25	D12S391	18	25	18	25
	D2S1338	19	21	D2S1338	19	21	19	21
			TPOX	8	8	8	8	
7	D3S1358	15	16	D3S1358	15	16	15	16
	vWA	17	18	vWA	17	18	17	18
	D16S539	11	12	D16S539	11	12	11	12
	CSF1PO	12	12	CSF1PO	12	12	12	12
	TPOX	8	8	D6S1043	12	12	12	12
	Yindel	2		Yindel	2		2	
	AMEL	X		AMEL	X		X	
	D8S1179	12	12	D8S1179	12	12	12	12
	D21S11	28	29	D21S11	28	29	28	29
	D18S51	12	14	D18S51	12	14	12	14
	DYS391	10	10	D5S818	12	12	12	12
	D2S441	12	12	D2S441	12	12	12	12
	D19S433	13	15.2	D19S433	13	15.2	13	15.2
	TH01	6	8	FGA	21	21	21	21

Table 16: Concordance study with blood and buccal swab samples using GlobalFiler (GF) and Verifiler Plus (VFP) PCR kits (continued)

Sample	markers	GF		markers	VFP- Blood		VFP- Buccal swab	
	FGA	21	21	D10S1248	14	14	14	14
	D22S1045	11	17	D22S1045	11	17	11	17
	D5S818	12	12	D1S1656	12	16	12	16
	D13S317	11	13	D13S317	11	13	11	13
	D7S820	10	11	D7S820	10	11	10	11
	SE33	27.2	28.2	Penta E	7	7	7	7
	D10S1248	14	14	Penta D	8	12	8	12
	D1S1656	12	16	TH01	6	8	6	8
	D12S391	19	21	D12S391	19	21	19	21
	D2S1338	21	22	D2S1338	21	22	21	22
				TPOX	8	8	8	8
	D3S1358	15	16	D3S1358	15	16	15	16
	vWA	16	18	vWA	16	18	16	18
	D16S539	9	11	D16S539	9	11	9	11
	CSF1PO	11	12	CSF1PO	11	12	11	12
	TPOX	8	11	D6S1043	11	11	11	11
8	Yindel			Yindel				
	AMEL	X	X	AMEL	x	x	X	x
	D8S1179	16	17	D8S1179	16	17	16	17
	D21S11	32.2	32.2	D21S11	32.2	32.2	32.2	32.2
	D18S51	14	15	D18S51	14	15	14	15
	DYS391			D5S818	11	12	11	12
	D2S441	14	14	D2S441	14	14	14	14
	D19S433	13	14	D19S433	13	14	13	14
	TH01	6	7	FGA	20	21	20	21
	FGA	20	21	D10S1248	14	15	14	15
	D22S1045	15	15	D22S1045	15	15	15	15
	D5S818	11	12	D1S1656	15	16	15	16
	D13S317	11	11	D13S317	11	11	11	11
	D7S820	10	10	D7S820	10	10	10	10
	SE33	14	29.2	Penta E	13	13	13	13
	D10S1248	14	15	Penta D	11	11	11	11
	D1S1656	15	16	TH01	6	7	6	7
	D12S391	20	20	D12S391	20	20	20	20
	D2S1338	19	23	D2S1338	19	23	19	23
				TPOX	8	11	8	11
9	D3S1358	15	17	D3S1358	15	17	15	17
	vWA	18	19	vWA	18	19	18	19
	D16S539	11	13	D16S539	11	13	11	13
	CSF1PO	11	12	CSF1PO	11	12	11	12
	TPOX	8	9	D6S1043	11	19	11	19

Table 16: Concordance study with blood and buccal swab samples using GlobalFiler (GF) and Verifiler Plus (VFP) PCR kits (continued)

Sample	GF		markers	VFP- Blood		VFP- Buccal swab	
	markers						
	Yindel	2	Yindel	2		2	
	AMEL	X	Y	AMEL	X	Y	X
	D8S1179	13	14	D8S1179	13	14	13
	D21S11	30	34.2	D21S11	30	34.2	30
	D18S51	12	14	D18S51	12	14	12
	DYS391	11		D5S818	11	13	11
	D2S441	11	14	D2S441	11	14	11
	D19S433	12	16.2	D19S433	12	16.2	12
	TH01	6	7	FGA	24	24	24
	FGA	24	24	D10S1248	15	15	15
	D22S1045	15	15	D22S1045	15	15	15
	D5S818	11	13	D1S1656	15	17	15
	D13S317	11	12	D13S317	11	12	11
	D7S820	8	10	D7S820	8	10	8
	SE33	27.2	33	Penta E	7	14	7
	D10S1248	15	15	Penta D	12	13	12
	D1S1656	15	17	TH01	6	7	6
	D12S391	15	22	D12S391	15	22	15
	D2S1338	18	24	D2S1338	18	24	18
				TPOX	8	9	8
10	D3S1358	16	17	D3S1358	16	17	16
	vWA	13	14	vWA	13	14	13
	D16S539	9	11	D16S539	9	11	9
	CSF1PO	11	12	CSF1PO	11	12	11
	TPOX	8	11	D6S1043	11	13	11
	Yindel	2		Yindel	2		2
	AMEL	X	Y	AMEL	X	Y	X
	D8S1179	13	14	D8S1179	13	14	13
	D21S11	27	30	D21S11	27	30	27
	D18S51	15	19	D18S51	15	19	15
	DYS391	10		D5S818	12	12	12
	D2S441	11	14	D2S441	11	14	11
	D19S433	15	15.2	D19S433	15	15.2	15
	TH01	7	9	FGA	21	23	21
	FGA	21	23	D10S1248	14	14	14
	D22S1045	14	15	D22S1045	14	15	14
	D5S818	12	12	D1S1656	11	11	11
	D13S317	12	12	D13S317	12	12	12
	D7S820	10	11	D7S820	10	11	10
	SE33	17	35.2	Penta E	17	18	17
	D10S1248	14	14	Penta D	9	14	9

Table 16: Concordance study with blood and buccal swab samples using GlobalFiler (GF) and Verifiler Plus (VFP) PCR kits (continued)

Sample	markers	GF		markers	VFP- Blood		VFP- Buccal swab	
	D1S1656	11	11	TH01	7	9	7	9
	D12S391	22	24	D12S391	22	24	22	24
	D2S1338	17	17	D2S1338	17	17	17	17
				TPOX	8	11	8	11
11	D3S1358	15	17	D3S1358	15	17	15	17
	vWA	17	18	vWA	17	18	17	18
	D16S539	11	12	D16S539	11	12	11	12
	CSF1PO	10	12	CSF1PO	10	12	10	12
	TPOX	8	9	D6S1043	12	17	12	17
	Yindel	2		Yindel	2		2	
	AMEL	X	Y	AMEL	X	Y	X	Y
	D8S1179	13	14	D8S1179	13	14	13	14
	D21S11	29	31	D21S11	29	31	29	31
	D18S51	13	18	D18S51	13	18	13	18
	DYS391	10		D5S818	12	13	12	13
	D2S441	11	14	D2S441	11	14	11	14
	D19S433	14	14.2	D19S433	14	14.2	14	14.2
	TH01	9	9	FGA	21	26	21	26
	FGA	21	26	D10S1248	13	15	13	15
	D22S1045	16	16	D22S1045	16	16	16	16
	D5S818	12	13	D1S1656	16	16.3	16	16.3
	D13S317	13	13	D13S317	13	13	13	13
	D7S820	10	10	D7S820	10	10	10	10
	SE33	17	20	Penta E	17	18	17	18
	D10S1248	13	15	Penta D	9	14	9	14
	D1S1656	16	16.3	TH01	9	9	9	9
	D12S391	22	22	D12S391	22	22	22	22
	D2S1338	20	21	D2S1338	20	22	20	22
				TPOX	8	9	8	9
12	D3S1358	16	18	D3S1358	16	18	16	18
	vWA	15	16	vWA	15	16	15	16
	D16S539	12	12	D16S539	12	12	12	12
	CSF1PO	5	11	CSF1PO	5	11	5	11
	TPOX	8	9	D6S1043	12	19	12	19
	Yindel	2		Yindel	2		2	
	AMEL	X	Y	AMEL	X	Y	X	Y
	D8S1179	14	14	D8S1179	14	14	14	14
	D21S11	29	31	D21S11	29	31	29	31
	D18S51	13	15	D18S51	13	15	13	15
	DYS391	11		D5S818	9	12	9	12
	D2S441	11	14	D2S441	11	14	11	14

Table 16: Concordance study with blood and buccal swab samples using GlobalFiler (GF) and Verifiler Plus (VFP) PCR kits (continued)

Sample	markers	GF		markers	VFP- Blood		VFP- Buccal swab	
	D19S433	13	14	D19S433	13	14	13	14
	TH01	6	9	FGA	23	24	23	24
	FGA	23	24	D10S1248	15	16	15	16
	D22S1045	15	15	D22S1045	15	15	15	15
	D5S818	9	12	D1S1656	15.3	16	15.3	16
	D13S317	8	11	D13S317	8	11	8	11
	D7S820	9	11	D7S820	9	11	9	11
	SE33	14	17	Penta E	11	13	11	13
	D10S1248	15	16	Penta D	9	15	9	15
	D1S1656	15.3	16	TH01	6	9	6	9
	D12S391	18	24	D12S391	18	24	18	24
	D2S1338	16	20	D2S1338	16	20	16	20
				TPOX	8	9	8	9
	D1S1656	15.3	16	TH01	6	9	6	9
	D12S391	18	24	D12S391	18	24	18	24
	D2S1338	16	20	D2S1338	16	20	16	20
				TPOX	8	9	8	9
13	D3S1358	15	18	D3S1358	15	18	15	18
	vWA	16	16	vWA	16	16	16	16
	D16S539	10	12	D16S539	10	12	10	12
	CSF1PO	11	11	CSF1PO	11	11	11	11
	TPOX	9	10	D6S1043	11	12	11	12
	Yindel	2		Yindel	2		2	
	AMEL	X	Y	AMEL	X	Y	X	Y
	D8S1179	14	16	D8S1179	14	16	14	16
	D21S11	28	30	D21S11	28	30	28	30
	D18S51	14	16	D18S51	14	16	14	16
	DYS391	10		D5S818	10	12	10	12
	D2S441	14	14	D2S441	14	14	14	14
	D19S433	12	13.2	D19S433	12	13.2	12	13.2
	TH01	9	9	FGA	21	24	21	24
	FGA	21	24	D10S1248	14	15	14	15
	D22S1045	15	16	D22S1045	15	16	15	16
	D5S818	10	12	D1S1656	11	11	11	11
	D13S317	11	11	D13S317	11	11	11	11
	D7S820	11	13	D7S820	11	13	11	13
	SE33	30.2	31.2	Penta E	9	12	9	12
	D10S1248	14	15	Penta D	12	12	12	12
	D1S1656	11	11	TH01	9	9	9	9
	D12S391	24	26	D12S391	24	26	24	26
	D2S1338	17	20	D2S1338	17	20	17	20

Table 16: Concordance study with blood and buccal swab samples using GlobalFiler (GF) and Verifiler Plus (VFP) PCR kits (continued)

Sample	markers	GF		markers	VFP- Blood		VFP- Buccal swab	
				TPOX	9	10	9	10
14	D3S1358	16	17	D3S1358	16	17	16	17
	vWA	15	16	vWA	15	16	15	16
	D16S539	11	14	D16S539	11	14	11	14
	CSF1PO	11	13	CSF1PO	11	13	11	13
	TPOX	9	9	D6S1043	11	14	11	14
	Yindel			Yindel				
	AMEL	X	X	AMEL	X	X	X	X
	D8S1179	10	13	D8S1179	10	13	10	13
	D21S11	30	32.2	D21S11	30	32.2	30	32.2
	D18S51	13	18	D18S51	13	18	13	18
	DYS391			D5S818	11	11	11	11
	D2S441	11	14	D2S441	11	14	11	14
	D19S433	13	15	D19S433	13	15	13	15
	TH01	6	9	FGA	22	24	22	24
	FGA	22	24	D10S1248	14	14	14	14
	D22S1045	11	12	D22S1045	11	12	11	12
	D5S818	11	11	D1S1656	12	16	12	16
	D13S317	10	12	D13S317	10	12	10	12
	D7S820	9	11	D7S820	9	11	9	11
	SE33	27.2	32.2	Penta E	11	12	11	12
	D10S1248	14	14	Penta D	13	14	13	14
	D1S1656	12	16	TH01	6	9	6	9
	D12S391	20	21	D12S391	20	21	20	21
D2S1338	20	21	D2S1338	20	21	20	21	
			TPOX	9	9	9	9	
15	D3S1358	15	16	D3S1358	15	16	15	16
	vWA	16	16	vWA	16	16	16	16
	D16S539	11	11	D16S539	11	11	11	11
	CSF1PO	12	12	CSF1PO	12	12	12	12
	TPOX	8	8	D6S1043	19	19	19	19
	Yindel			Yindel				
	AMEL	X	X	AMEL	X	X	X	X
	D8S1179	10	12	D8S1179	10	12	10	12
	D21S11	31	31.2	D21S11	31	31.2	31	31.2
	D18S51	16	16	D18S51	16	16	16	16
	DYS391			D5S818	11	12	11	12
	D2S441	11	15	D2S441	11	15	11	15
	D19S433	13	13	D19S433	13	13	13	13
	TH01	6	9	FGA	22	25	22	25
	FGA	22	25	D10S1248	13	16	13	16

Table 16: Concordance study with blood and buccal swab samples using GlobalFiler (GF) and Verifiler Plus (VFP) PCR kits (continued)

Sample	markers	GF	markers	VFP- Blood	VFP- Buccal swab
	D22S1045	11 16	D22S1045	11 16	11 16
	D5S818	11 12	D1S1656	13 14.2	13 14.2
	D13S317	11 12	D13S317	11 12	11 12
	D7S820	8 12	D7S820	8 12	8 12
	SE33	17 22	Penta E	11 20	11 20
	D10S1248	13 16	Penta D	10 12	10 12
	D1S1656	13 OL	TH01	6 9	6 9
	D12S391	17 20	D12S391	17 20	17 20
	D2S1338	17 23	D2S1338	17 23	17 23
			TPOX	8 8	8 8
16	D3S1358	15 18	D3S1358	15 18	15 18
	vWA	14 16	vWA	14 16	14 16
	D16S539	12 12	D16S539	12 12	12 12
	CSF1PO	10 12	CSF1PO	10 12	10 12
	TPOX	9 10	D6S1043	13 14	13 14
	Yindel	2	Yindel	2	2
	AMEL	X Y	AMEL	X Y	X Y
	D8S1179	12 13	D8S1179	12 13	12 13
	D21S11	28 29	D21S11	28 29	28 29
	D18S51	12 14	D18S51	12 14	12 14
	DYS391	10	D5S818	11 12	11 12
	D2S441	11 14	D2S441	11 14	11 14
	D19S433	13 15	D19S433	13 15	13 15
	TH01	7 9	FGA	20 25	20 25
	FGA	20 25	D10S1248	14 15	14 15
	D22S1045	15 15	D22S1045	15 15	15 15
	D5S818	11 12	D1S1656	13 16.3	13 16.3
	D13S317	8 10	D13S317	8 10	8 10
	D7S820	11 11	D7S820	11 11	11 11
	SE33	15 18	Penta E	12 20	12 20
	D10S1248	14 15	Penta D	2.2 9	2.2 9
	D1S1656	13 16.3	TH01	7 9	7 9
	D12S391	21 24	D12S391	21 24	21 24
	D2S1338	17 19	D2S1338	17 19	17 19
			TPOX	9 10	9 10

Note: Markers in red represent the difference between the two PCR kits.